

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
 Data File : BF128233.D
 Acq On : 13 May 2022 11:17
 Operator : CG\JU
 Sample : PB144784BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144784BL

Quant Time: May 14 00:55:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 14 00:51:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	84602	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	346020	20.000	ng	0.00
39) Acenaphthene-d10	9.928	164	202050	20.000	ng	0.00
64) Phenanthrene-d10	11.416	188	372423	20.000	ng	0.00
76) Chrysene-d12	14.063	240	296999	20.000	ng	0.00
86) Perylene-d12	15.557	264	231318	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.522	112	505902	95.326	ng	0.01
7) Phenol-d6	6.516	99	645197	91.916	ng	-0.01
23) Nitrobenzene-d5	7.451	82	692696	90.079	ng	-0.01
42) 2,4,6-Tribromophenol	10.722	330	202154	87.238	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	1130155	87.520	ng	0.00
79) Terphenyl-d14	13.010	244	1394557	88.107	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
Data File : BF128233.D
Acq On : 13 May 2022 11:17
Operator : CG\JU
Sample : PB144784BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144784BL


Quant Time: May 14 00:55:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 14 00:51:21 2022
Response via : Initial Calibration

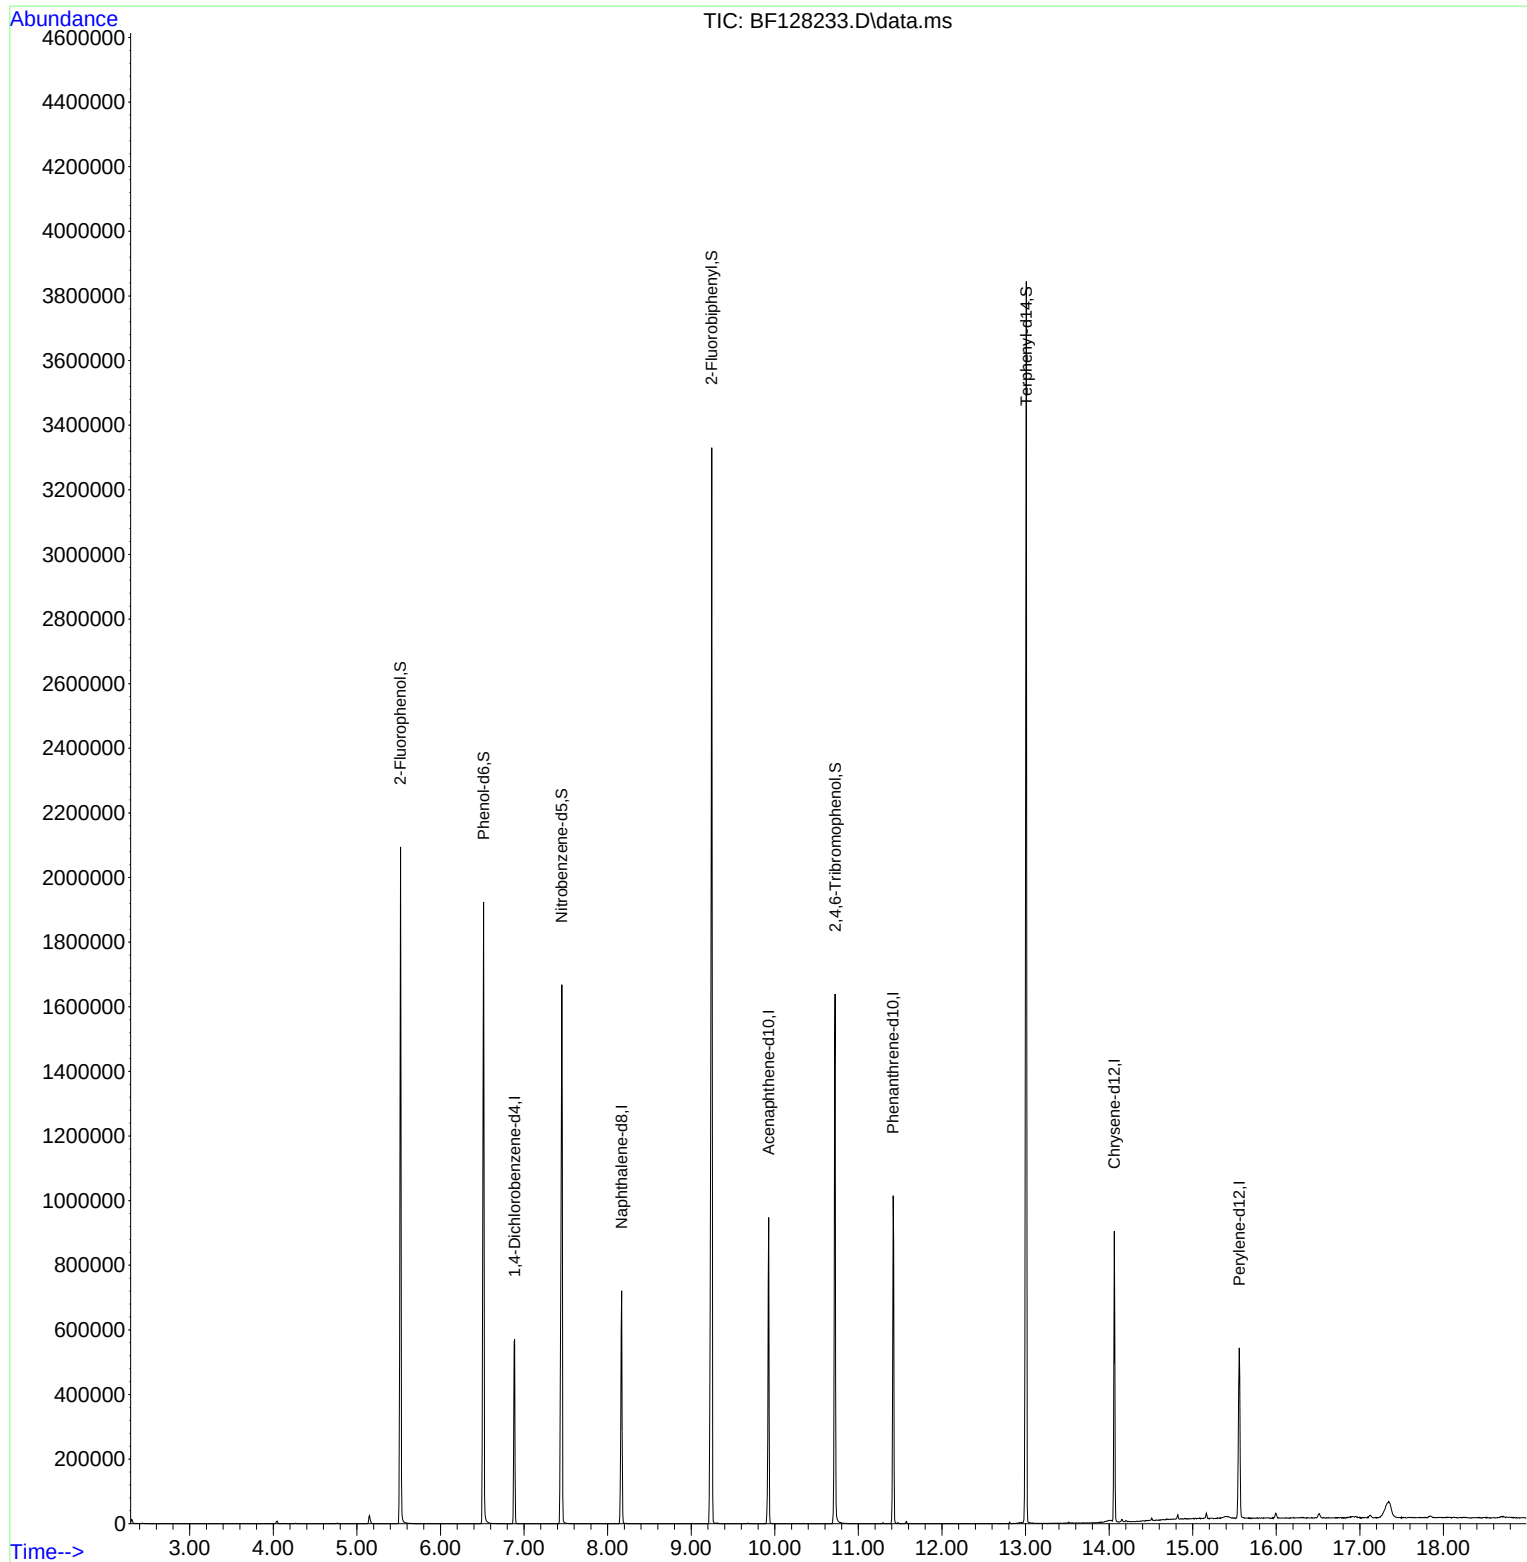



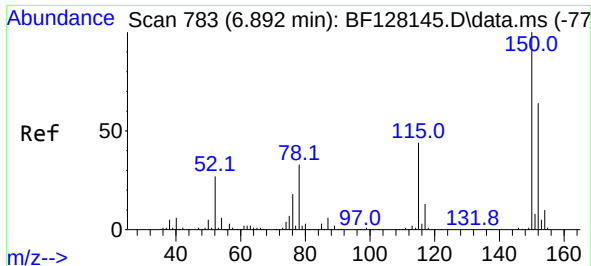


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.887 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF128233.D
Acq: 13 May 2022 11:17

Instrument :
BNA_F
ClientSampleId :
PB144784BL



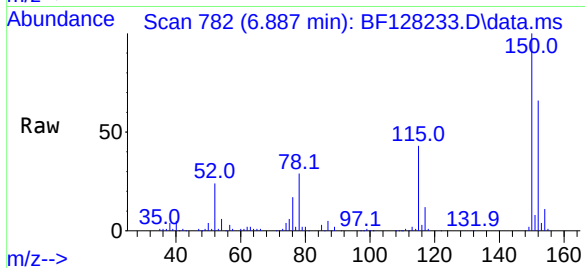



Tgt Ion:152 Resp: 84602
Ion Ratio Lower Upper
152 100
150 152.5 125.3 187.9
115 65.5 48.8 73.2

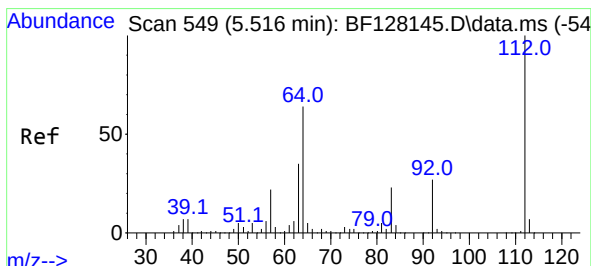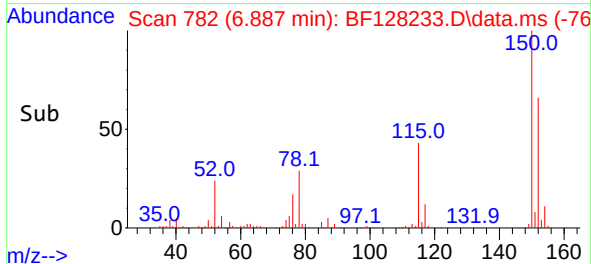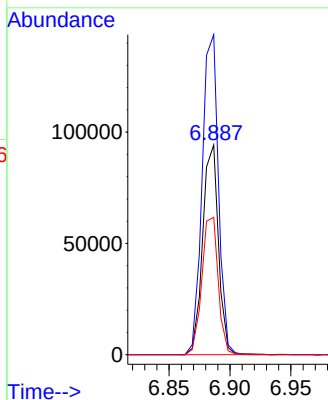

#5
2-Fluorophenol
Concen: 95.326 ng
RT: 5.522 min Scan# 550
Delta R.T. 0.012 min
Lab File: BF128233.D
Acq: 13 May 2022 11:17

Tgt Ion:112 Resp: 505902
Ion Ratio Lower Upper
112 100
64 68.5 49.5 74.3
63 37.5 26.3 39.5


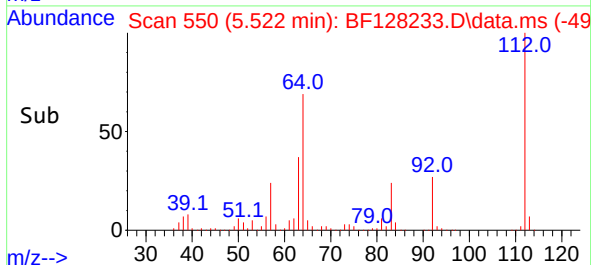
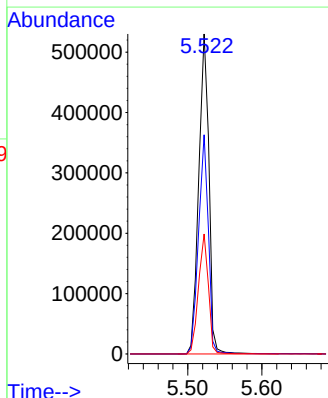
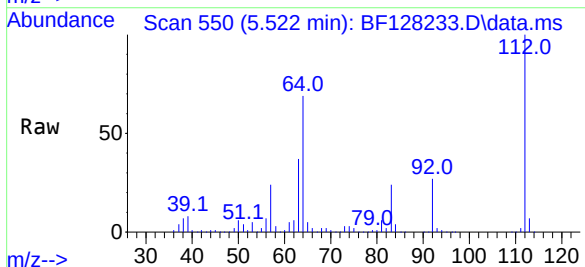


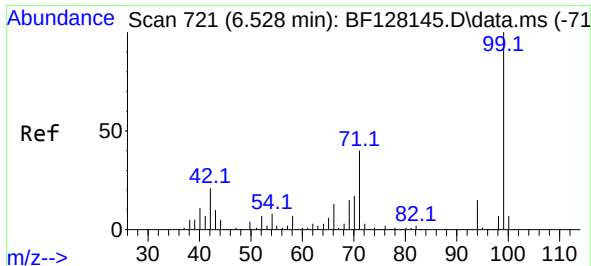

#7
Phenol-d6
Concen: 91.916 ng
RT: 6.516 min Scan# 71
Delta R.T. -0.012 min
Lab File: BF128233.D
Acq: 13 May 2022 11:17




Instrument :
BNA_F
ClientSampleId :
PB144784BL


Tgt Ion: 99 Resp: 645197
Ion Ratio Lower Upper
99 100
42 22.8 16.6 24.8
71 41.8 30.0 45.0

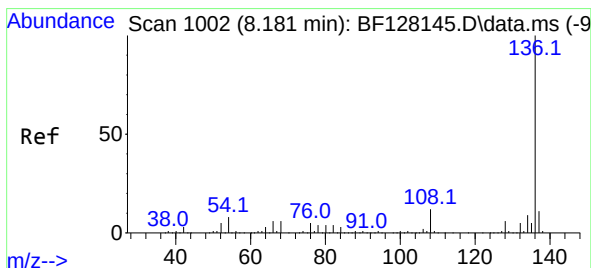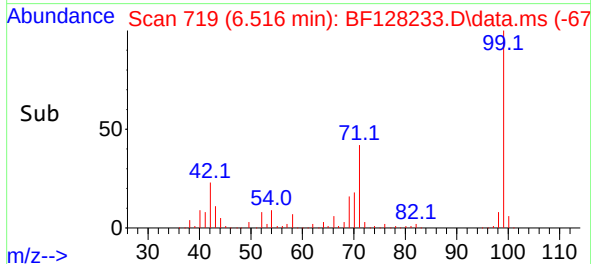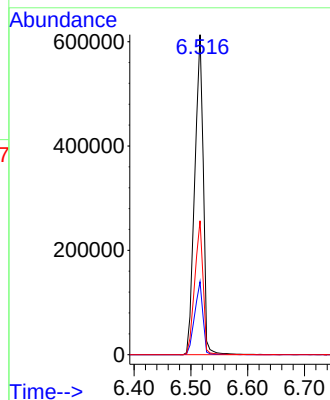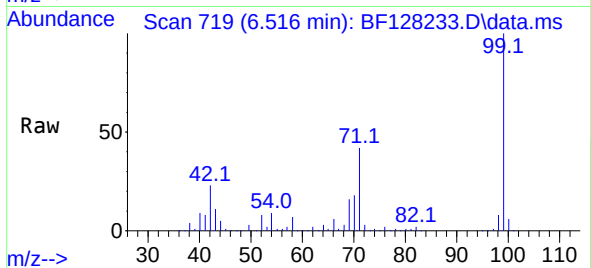

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1000
Delta R.T. -0.006 min
Lab File: BF128233.D
Acq: 13 May 2022 11:17


Tgt Ion: 136 Resp: 346020
Ion Ratio Lower Upper
136 100
137 10.4 8.6 13.0
54 8.3 6.8 10.2
68 5.6 5.1 7.7

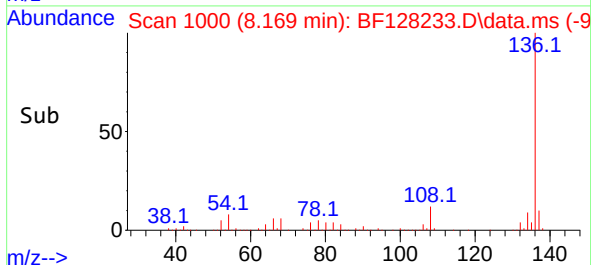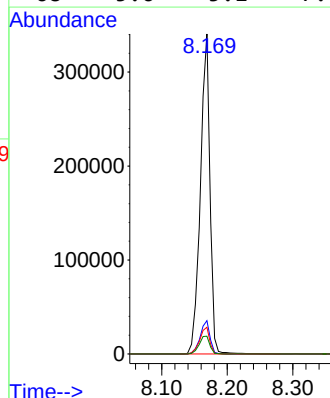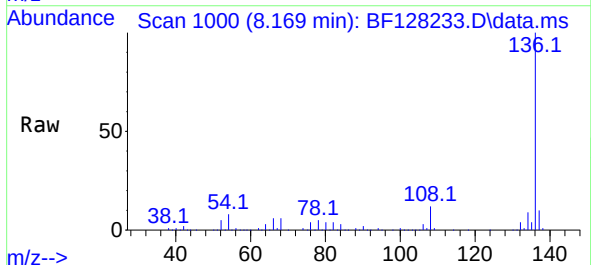



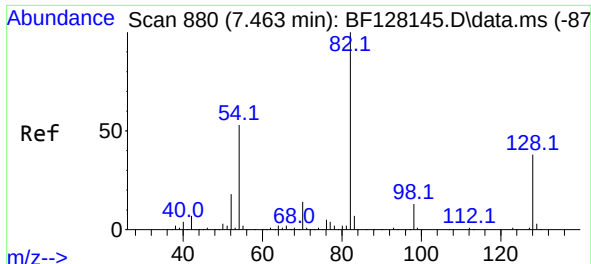


#23
Nitrobenzene-d5
Concen: 90.079 ng
RT: 7.451 min Scan# 81
Delta R.T. -0.012 min
Lab File: BF128233.D
Acq: 13 May 2022 11:17

Instrument :
BNA_F
ClientSampleId :
PB144784BL



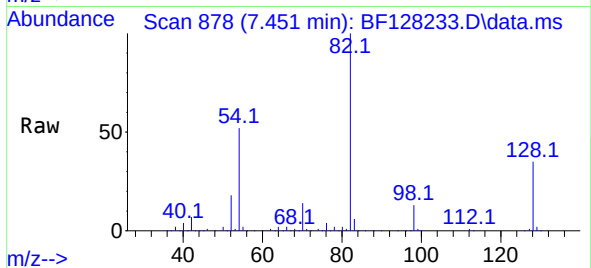



Tgt Ion: 82 Resp: 692696
Ion Ratio Lower Upper
82 100
128 35.4 30.0 45.0
54 52.3 41.3 61.9

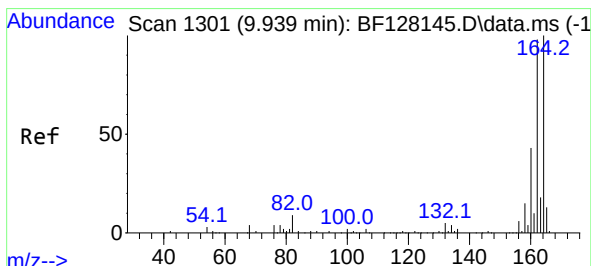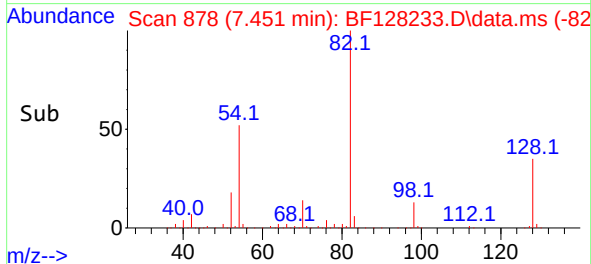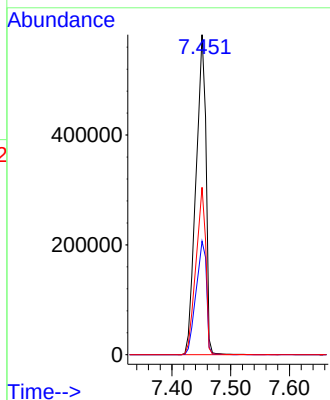

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.928 min Scan# 1299
Delta R.T. -0.006 min
Lab File: BF128233.D
Acq: 13 May 2022 11:17

Tgt Ion:164 Resp: 202050
Ion Ratio Lower Upper
164 100
162 95.8 76.0 114.0
160 43.9 34.8 52.2

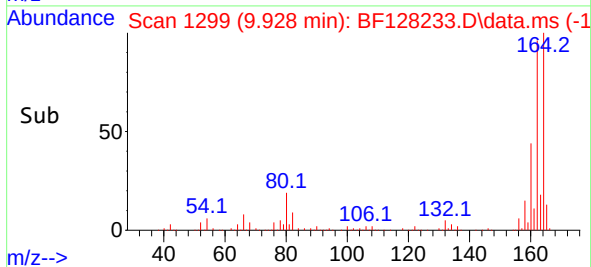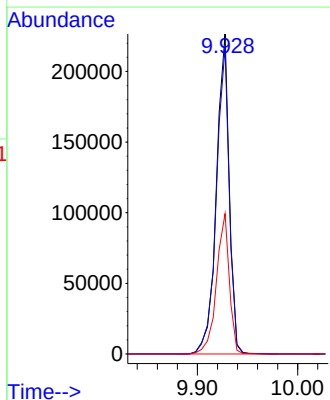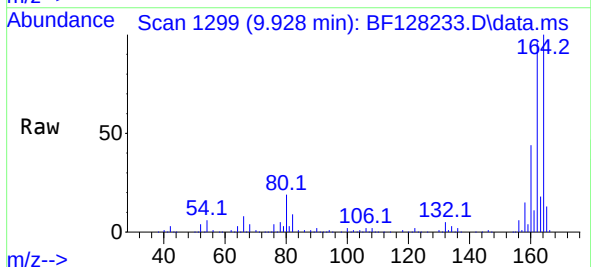

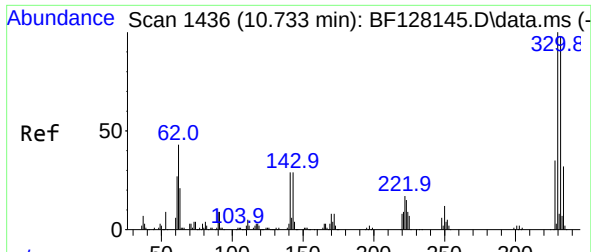

#42

2,4,6-Tribromophenol

Concen: 87.238 ng

RT: 10.722 min Scan# 1434

Delta R.T. -0.006 min

Lab File: BF128233.D

Acq: 13 May 2022 11:17

Instrument :

BNA_F

ClientSampleId :

PB144784BL





Tgt Ion:330 Resp: 202154

Ion Ratio Lower Upper

330 100

332 95.4 79.0 118.4

141 33.1 28.9 43.3

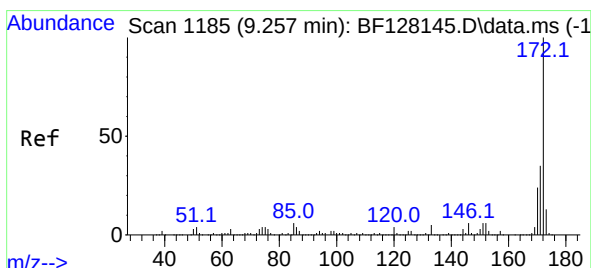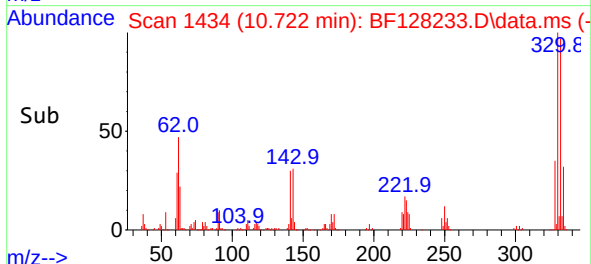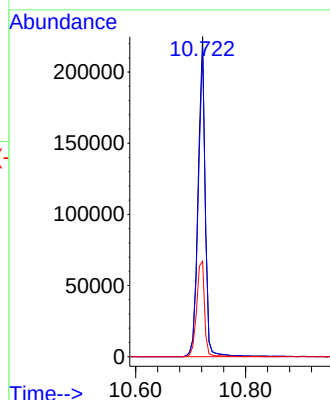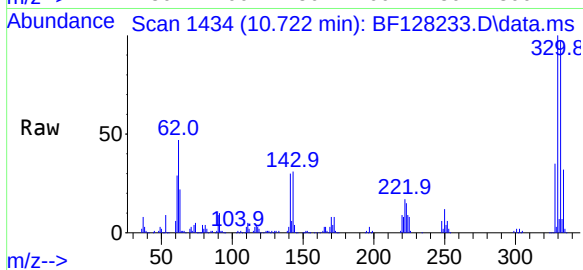

#45

2-Fluorobiphenyl

Concen: 87.520 ng

RT: 9.245 min Scan# 1183

Delta R.T. -0.006 min

Lab File: BF128233.D

Acq: 13 May 2022 11:17




Tgt Ion:172 Resp: 1130155


Ion Ratio Lower Upper

172 100

171 35.7 28.6 42.8

170 23.9 19.1 28.7


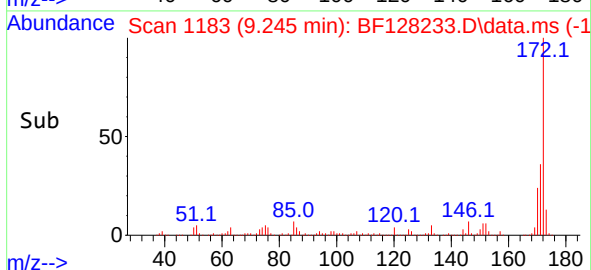
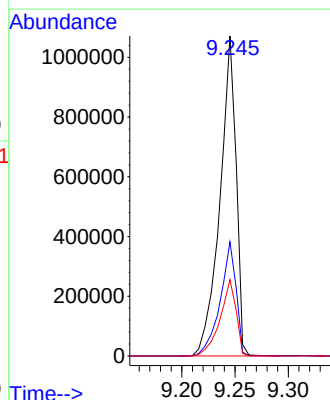
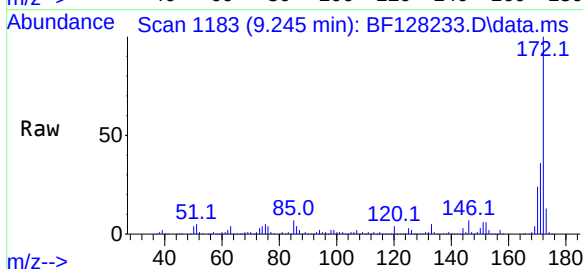


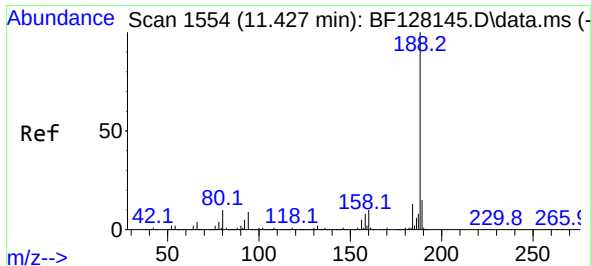

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.416 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF128233.D
Acq: 13 May 2022 11:17




Instrument :
BNA_F
ClientSampleId :
PB144784BL


Tgt Ion:188 Resp: 372423
Ion Ratio Lower Upper
188 100
94 9.4 8.0 12.0
80 10.5 8.9 13.3

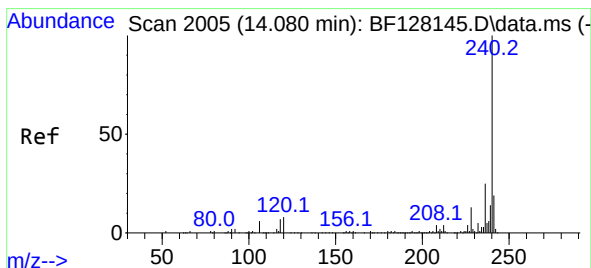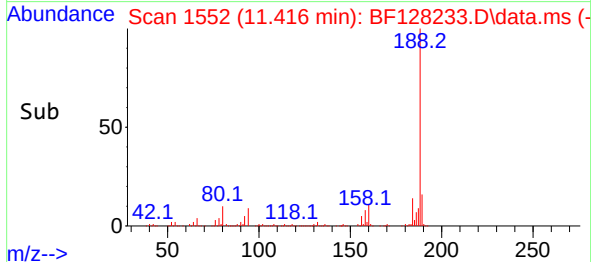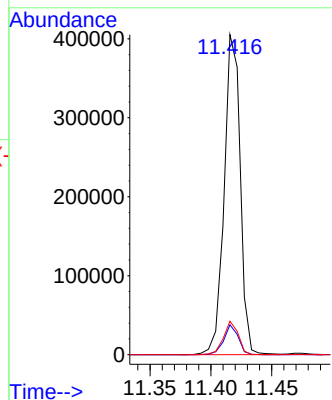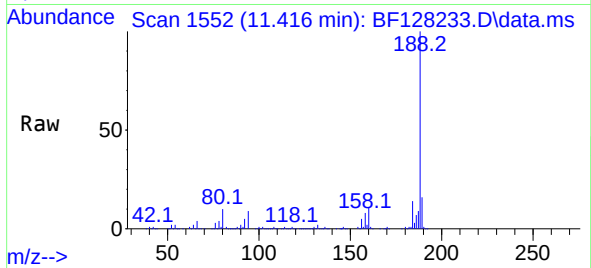

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.063 min Scan# 2002
Delta R.T. -0.006 min
Lab File: BF128233.D
Acq: 13 May 2022 11:17

Tgt Ion:240 Resp: 296999
Ion Ratio Lower Upper
240 100
120 9.5 7.0 10.6
236 25.0 20.3 30.5


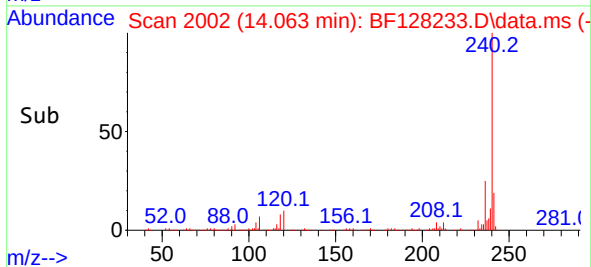
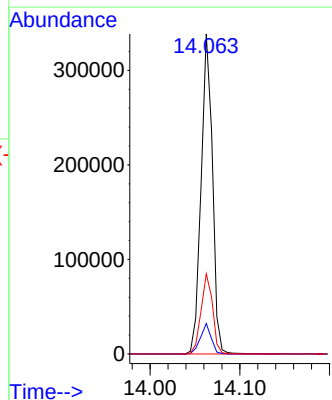
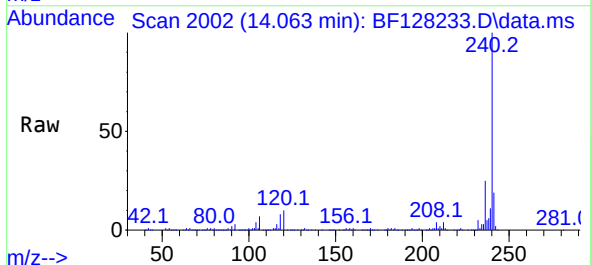


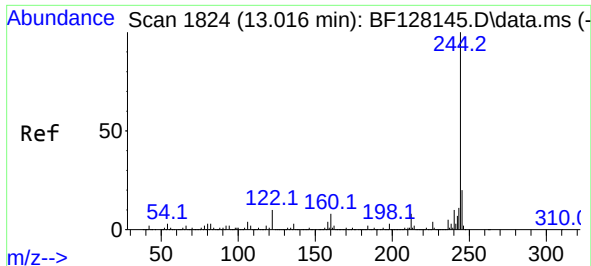

#79
 Terphenyl-d14
 Concen: 88.107 ng
 RT: 13.010 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BF128233.D
 Acq: 13 May 2022 11:17

Instrument :
 BNA_F
 ClientSampleId :
 PB144784BL

Tgt Ion:244 Resp: 1394557
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.2 9.4
 122 9.8 8.6 12.8

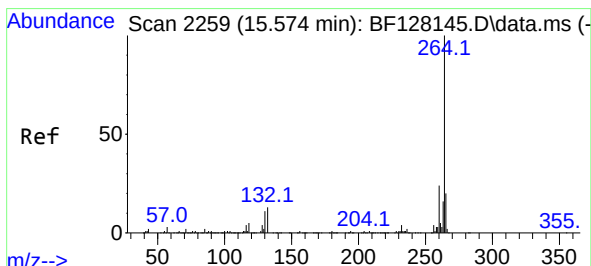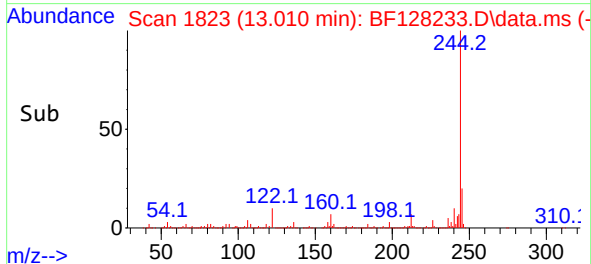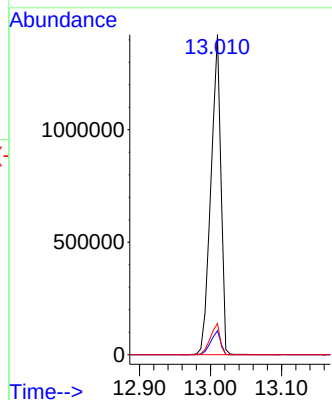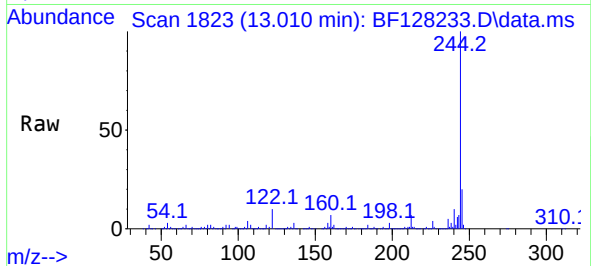

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.557 min Scan# 2256
 Delta R.T. -0.006 min
 Lab File: BF128233.D
 Acq: 13 May 2022 11:17

Tgt Ion:264 Resp: 231318
 Ion Ratio Lower Upper
 264 100
 260 24.3 20.1 30.1
 265 22.1 17.5 26.3

