

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
 Data File : BF128233.D
 Acq On : 13 May 2022 11:17
 Operator : CG\JU
 Sample : PB144784BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144784BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128233.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	546	550	553	rBV	2094156	1929598	51.85%	10.126%
2	6.516	714	719	722	rBV	1924047	1978820	53.17%	10.384%
3	6.887	778	782	785	rBV	571061	540246	14.52%	2.835%
4	7.451	872	878	881	rBV	1668353	1967289	52.86%	10.323%
5	8.169	994	1000	1003	rBV	721198	733619	19.71%	3.850%
6	9.245	1176	1183	1186	rBV	3330256	3418808	91.86%	17.940%
7	9.928	1292	1299	1302	rBV	947906	860355	23.12%	4.515%
8	10.722	1427	1434	1437	rBV	1639310	1554427	41.77%	8.157%
9	11.416	1546	1552	1556	rBV	1014842	912792	24.53%	4.790%
10	13.010	1817	1823	1826	rBV	3838916	3721592	100.00%	19.529%
11	14.063	1998	2002	2006	rBV	897245	781114	20.99%	4.099%
12	15.557	2250	2256	2263	rBV	526557	658076	17.68%	3.453%




Sum of corrected areas: 19056736

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
Data File : BF128233.D
Acq On : 13 May 2022 11:17
Operator : CG\JU
Sample : PB144784BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144784BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

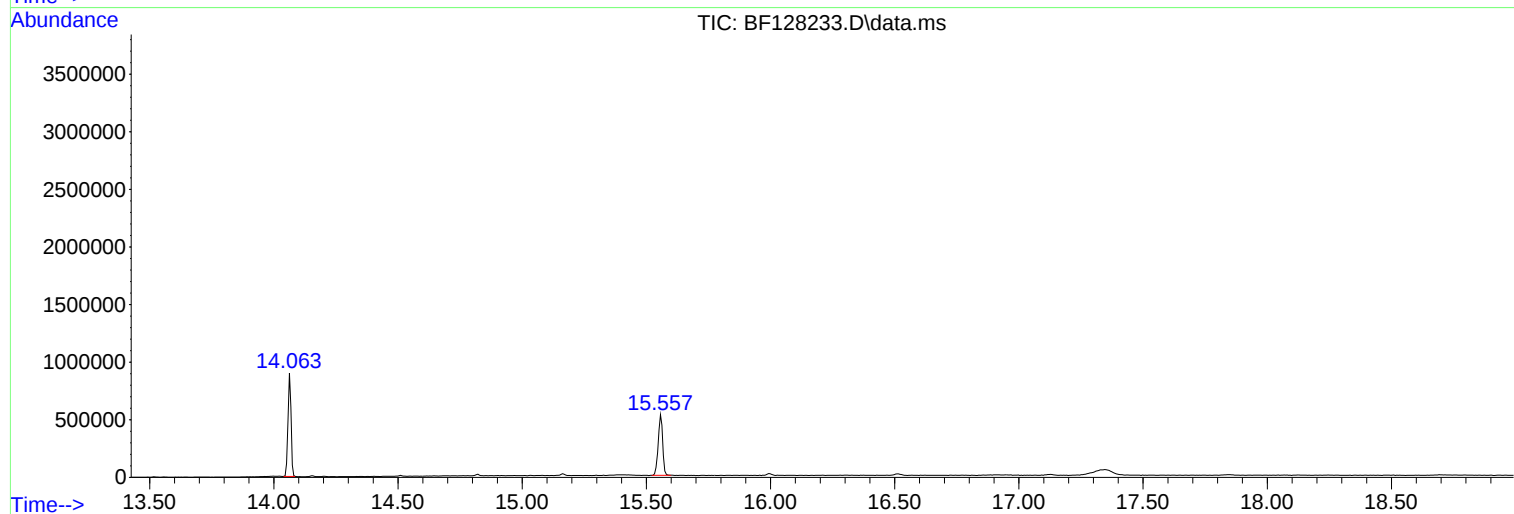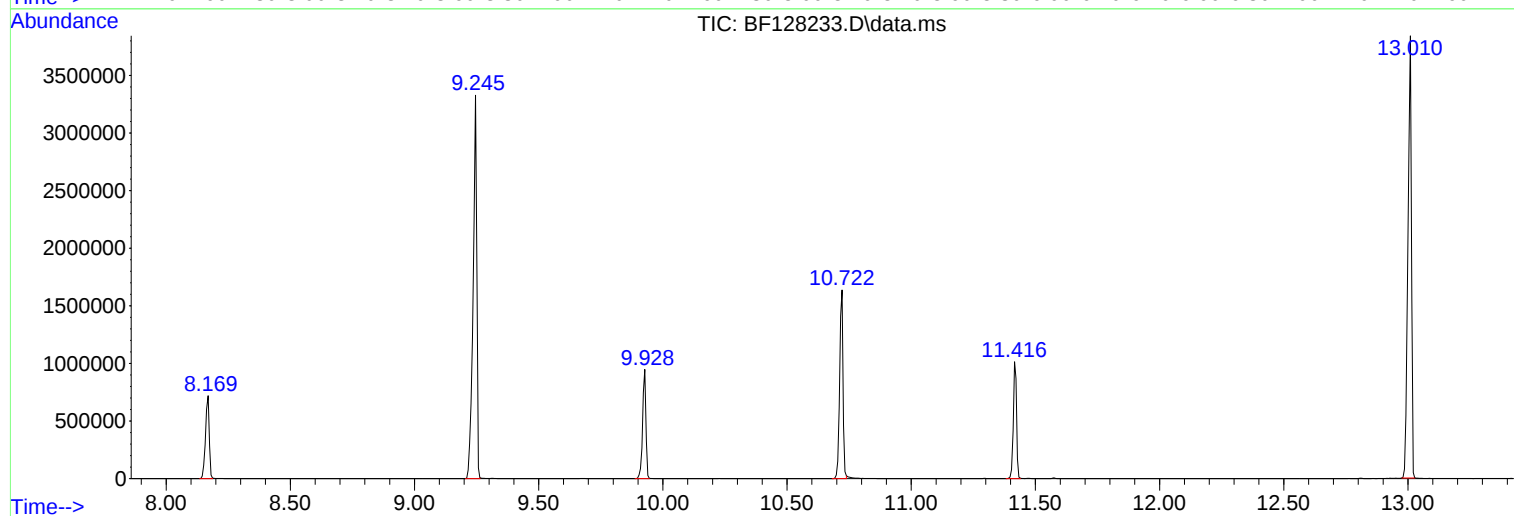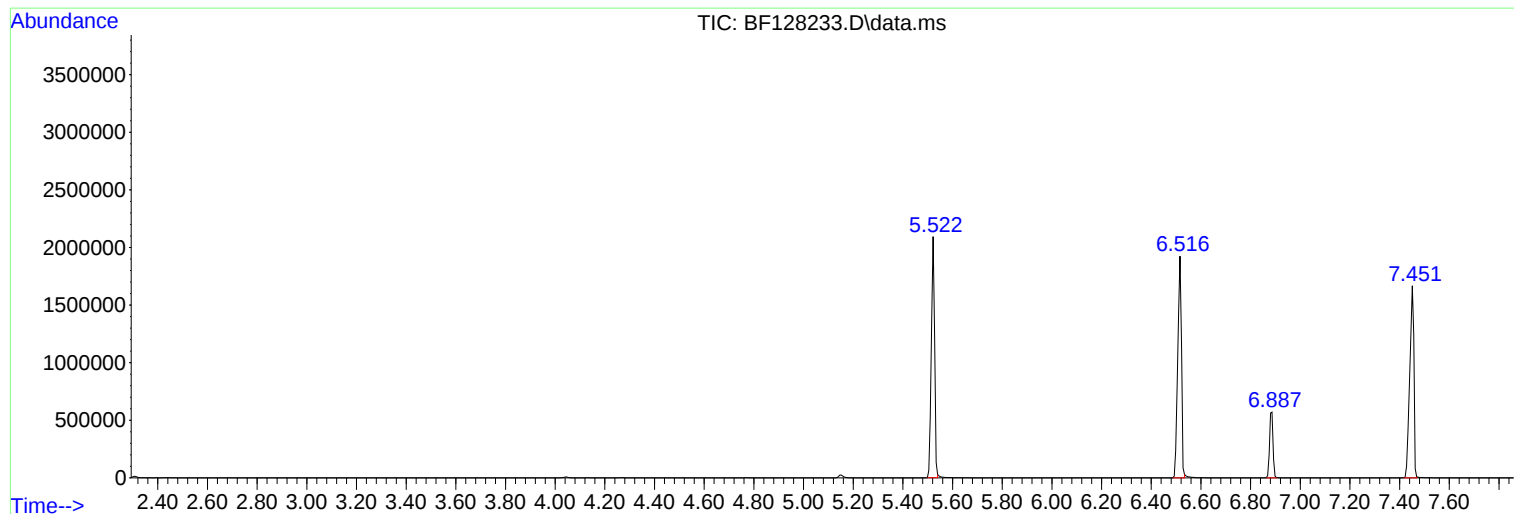

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
Data File : BF128233.D
Acq On : 13 May 2022 11:17
Operator : CG\JU
Sample : PB144784BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144784BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
Data File : BF128233.D
Acq On : 13 May 2022 11:17
Operator : CG\JU
Sample : PB144784BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144784BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------