

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
 Data File : BF128237.D
 Acq On : 13 May 2022 13:48
 Operator : CG\JU
 Sample : PB144757BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144757BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	546	551	554	rBV	2748467	2806304	74.87%	12.948%
2	6.522	714	720	723	rBV	2468631	2906140	77.53%	13.408%
3	6.881	778	781	785	rBV	626028	570622	15.22%	2.633%
4	7.451	872	878	881	rBV	1745977	1988132	53.04%	9.173%
5	8.169	994	1000	1003	rBV	682281	746153	19.91%	3.443%
6	9.245	1176	1183	1186	rBV	3308521	3510188	93.65%	16.195%
7	9.928	1292	1299	1302	rBV	879746	862797	23.02%	3.981%
8	10.722	1427	1434	1437	rBV	2409616	2259904	60.29%	10.427%
9	11.416	1546	1552	1556	rBV	1049202	914810	24.41%	4.221%
10	13.010	1815	1823	1826	rBV	3841143	3748370	100.00%	17.294%
11	14.063	1998	2002	2010	rVB	869510	765741	20.43%	3.533%
12	15.557	2250	2256	2262	rBV	469319	594824	15.87%	2.744%




Sum of corrected areas: 21673985

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
Data File : BF128237.D
Acq On : 13 May 2022 13:48
Operator : CG\JU
Sample : PB144757BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144757BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

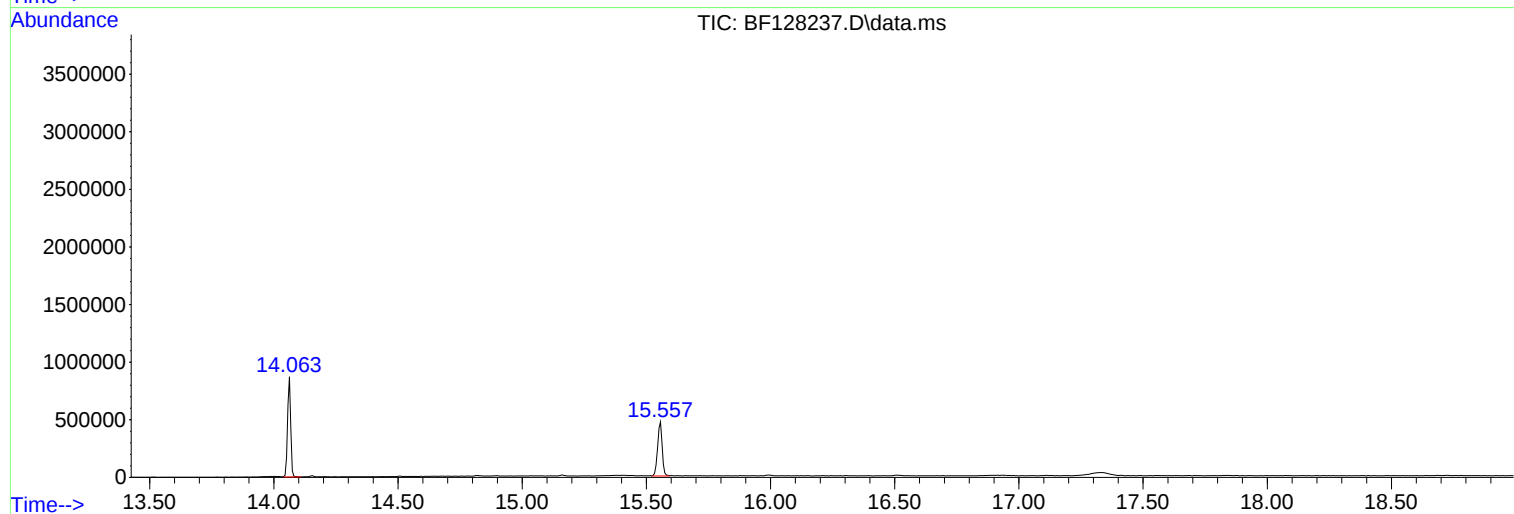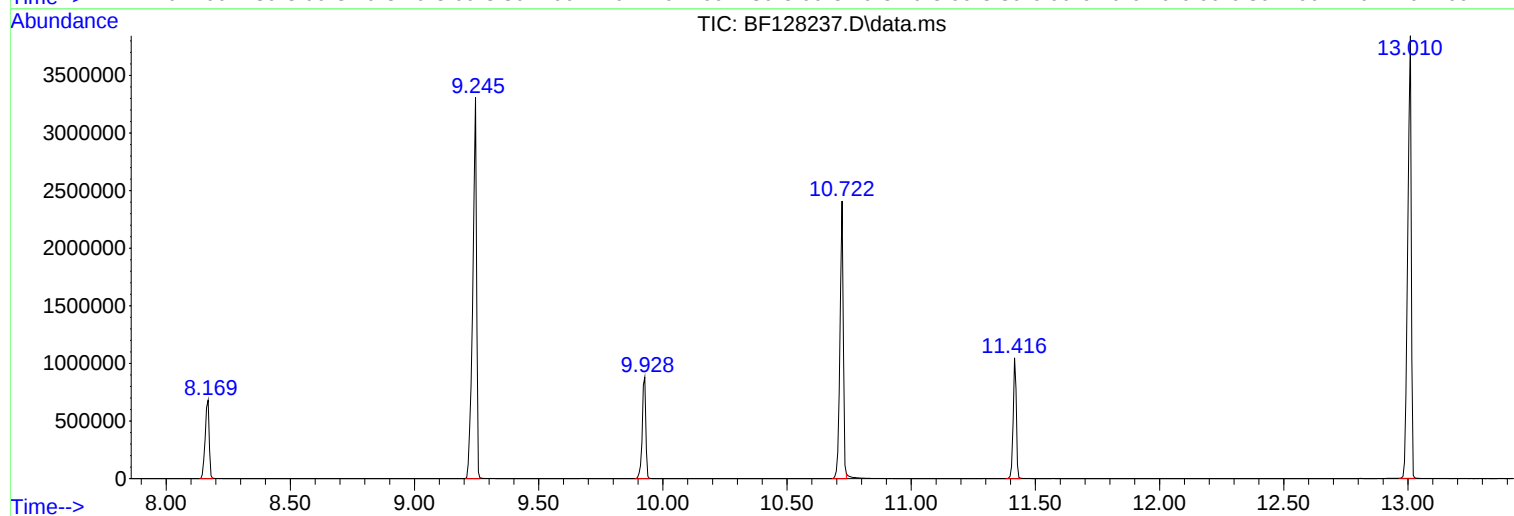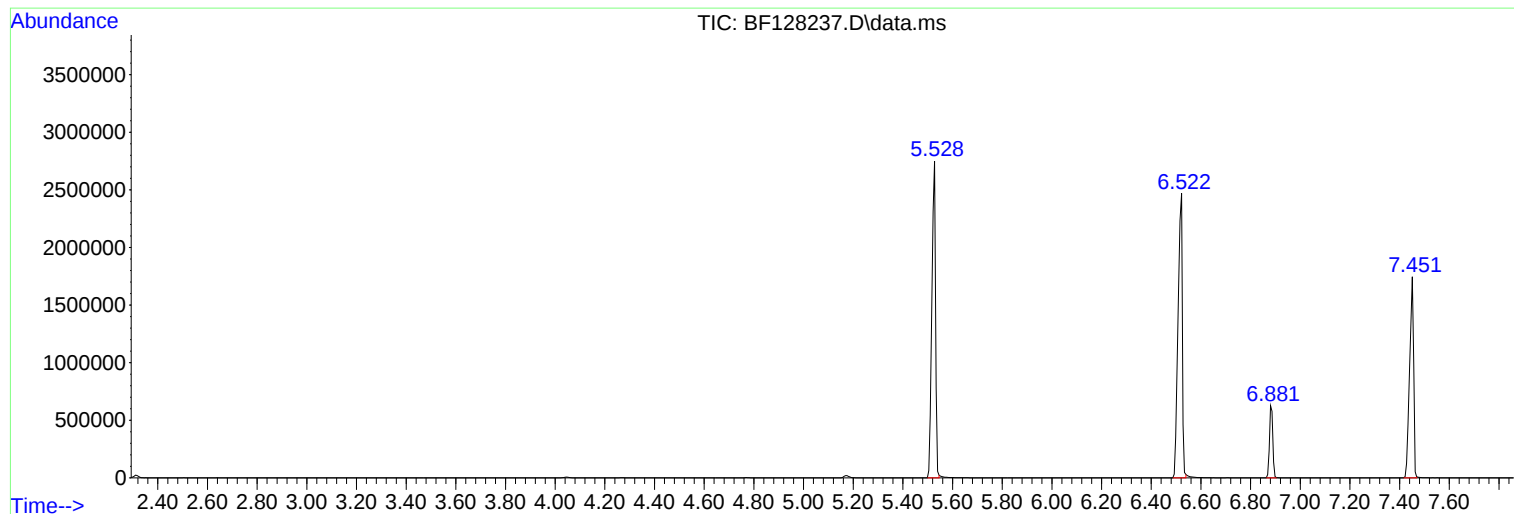

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
Data File : BF128237.D
Acq On : 13 May 2022 13:48
Operator : CG\JU
Sample : PB144757BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144757BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
Data File : BF128237.D
Acq On : 13 May 2022 13:48
Operator : CG\JU
Sample : PB144757BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144757BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------