
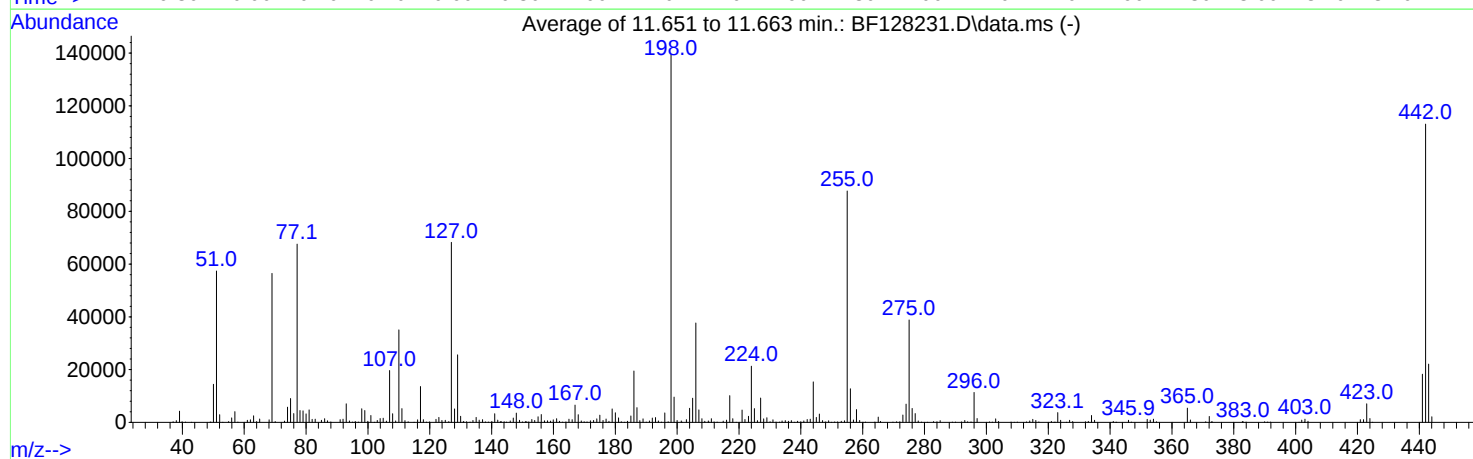


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051322\  
 Data File : BF128231.D  
 Acq On : 13 May 2022 10:20  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sat May 14 00:51:21 2022

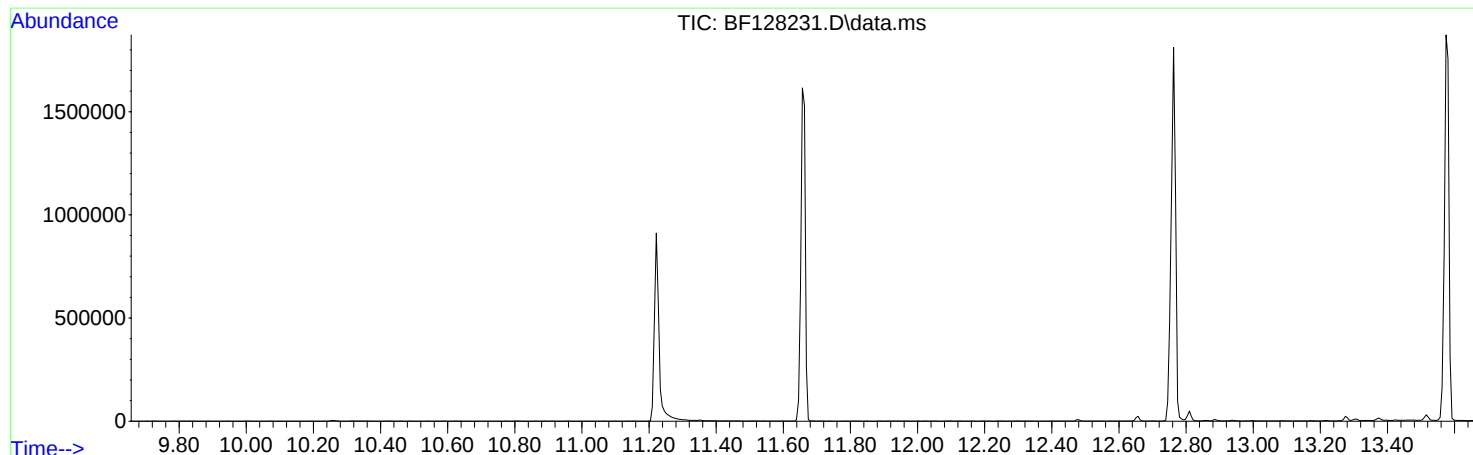




AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.2         | 57413      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 984        | PASS                |
| 69             | 198             | 0.00            | 100             | 40.5         | 56488      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 317        | PASS                |
| 127            | 198             | 10              | 80              | 48.9         | 68229      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.2          | 246        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 139445     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 9560       | PASS                |
| 275            | 198             | 10              | 60              | 27.8         | 38808      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 5386       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.1         | 18269      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 113053     | PASS                |
| 443            | 442             | 15              | 24              | 19.5         | 22084      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051322\  
 Data File : BF128231.D  
 Acq On : 13 May 2022 10:20  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: May 14 05:42:40 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Sat May 14 00:51:21 2022  
 Response via : Initial Calibration

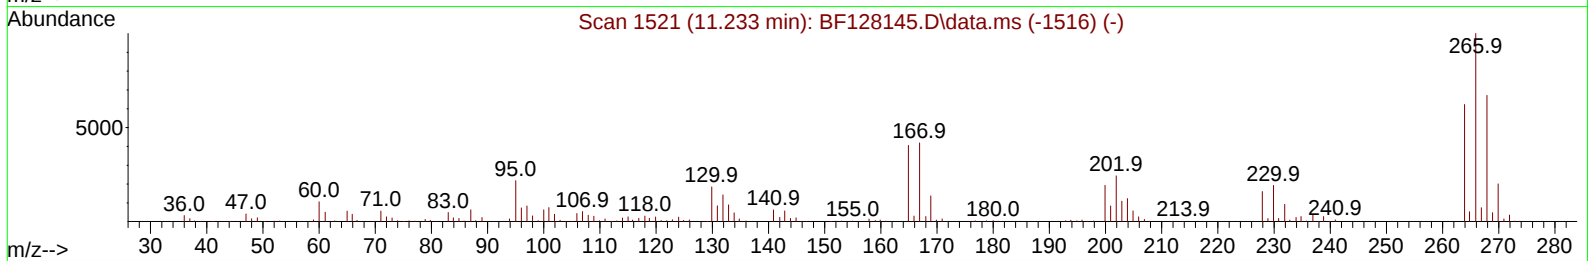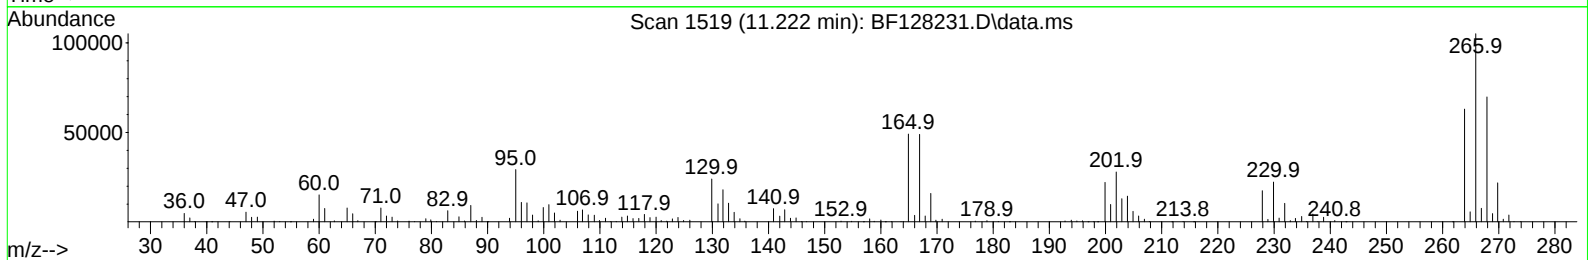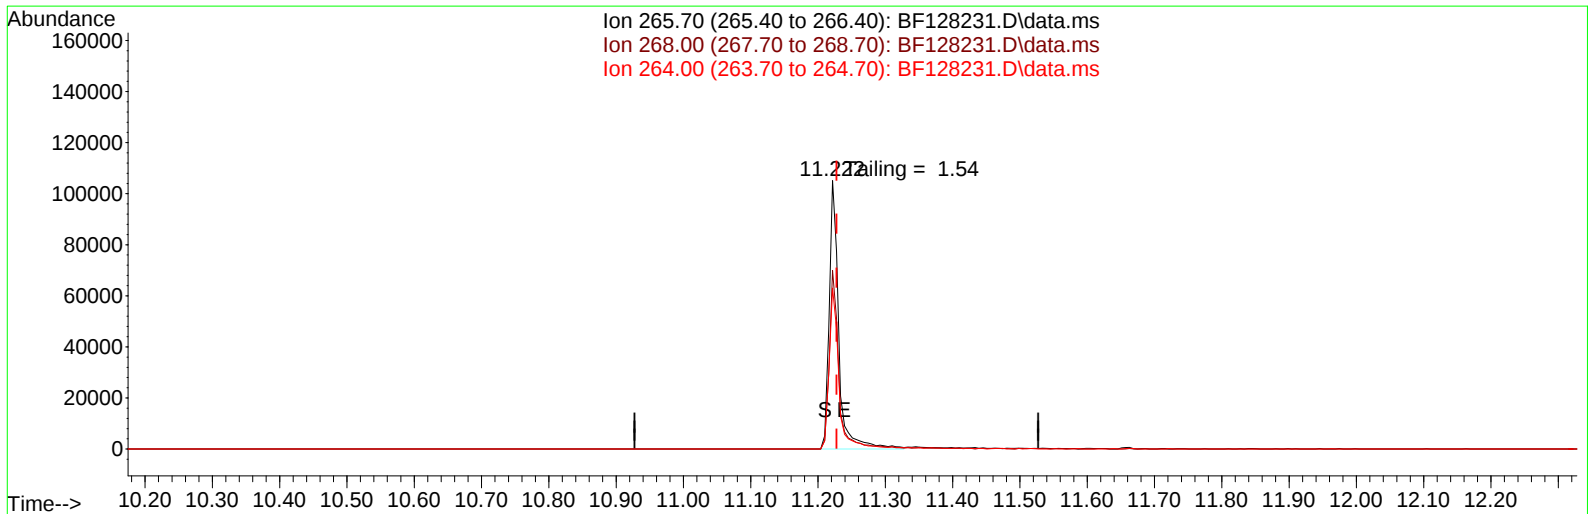

TIC: BF128231.D\data.ms

**(70) Pentachlorophenol (C)**

11.222min (-0.006) 26508.52 ng




response 104774

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.30  | 66.48  |
| 264.00 | 66.40  | 59.98  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051322\  
Data File : BF128231.D  
Acq On : 13 May 2022 10:20  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 14 05:42:40 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat May 14 00:51:21 2022  
Response via : Initial Calibration

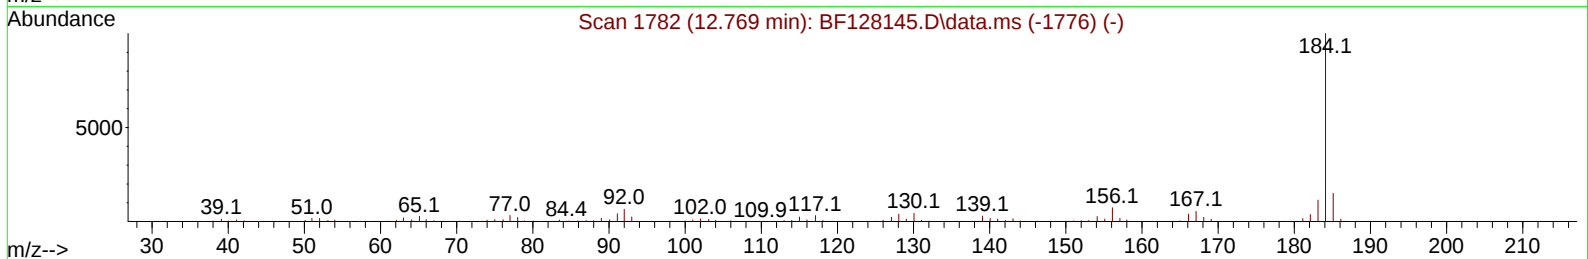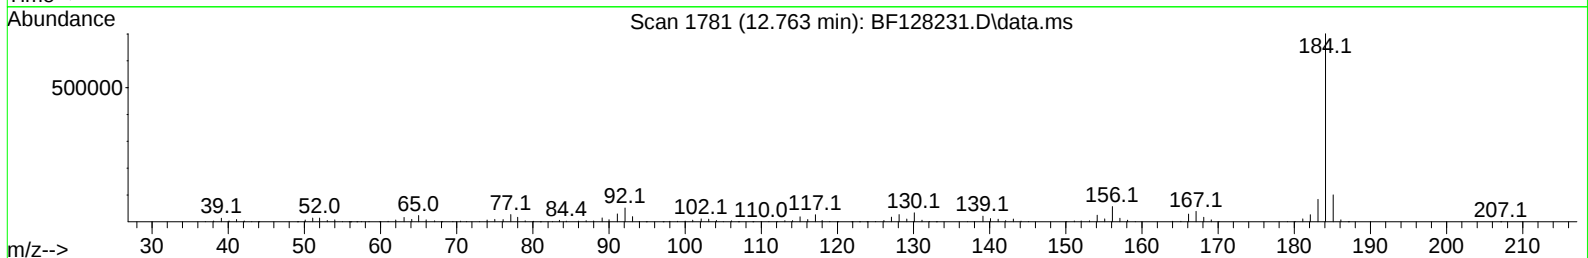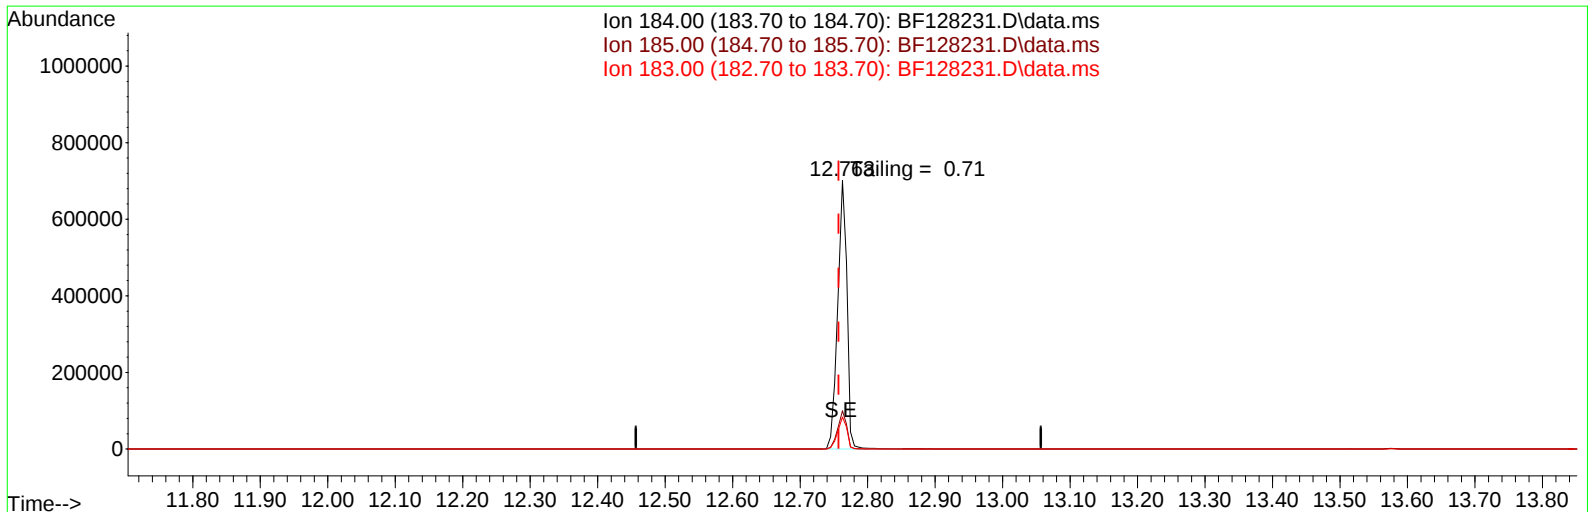

TIC: BF128231.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 671545

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.10  | 14.28  |
| 183.00 | 11.20  | 11.96  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/13/2022     | BNA_F            | <u>BF128231.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 338187           | 13.58              |
| DDD           | 6262             | 13.275             |
| DDE           | 652              | 12.939             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 6914          | 345101           | 2.00               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP