


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
 Data File : BF128235.D
 Acq On : 13 May 2022 12:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 14 00:51:21 2022

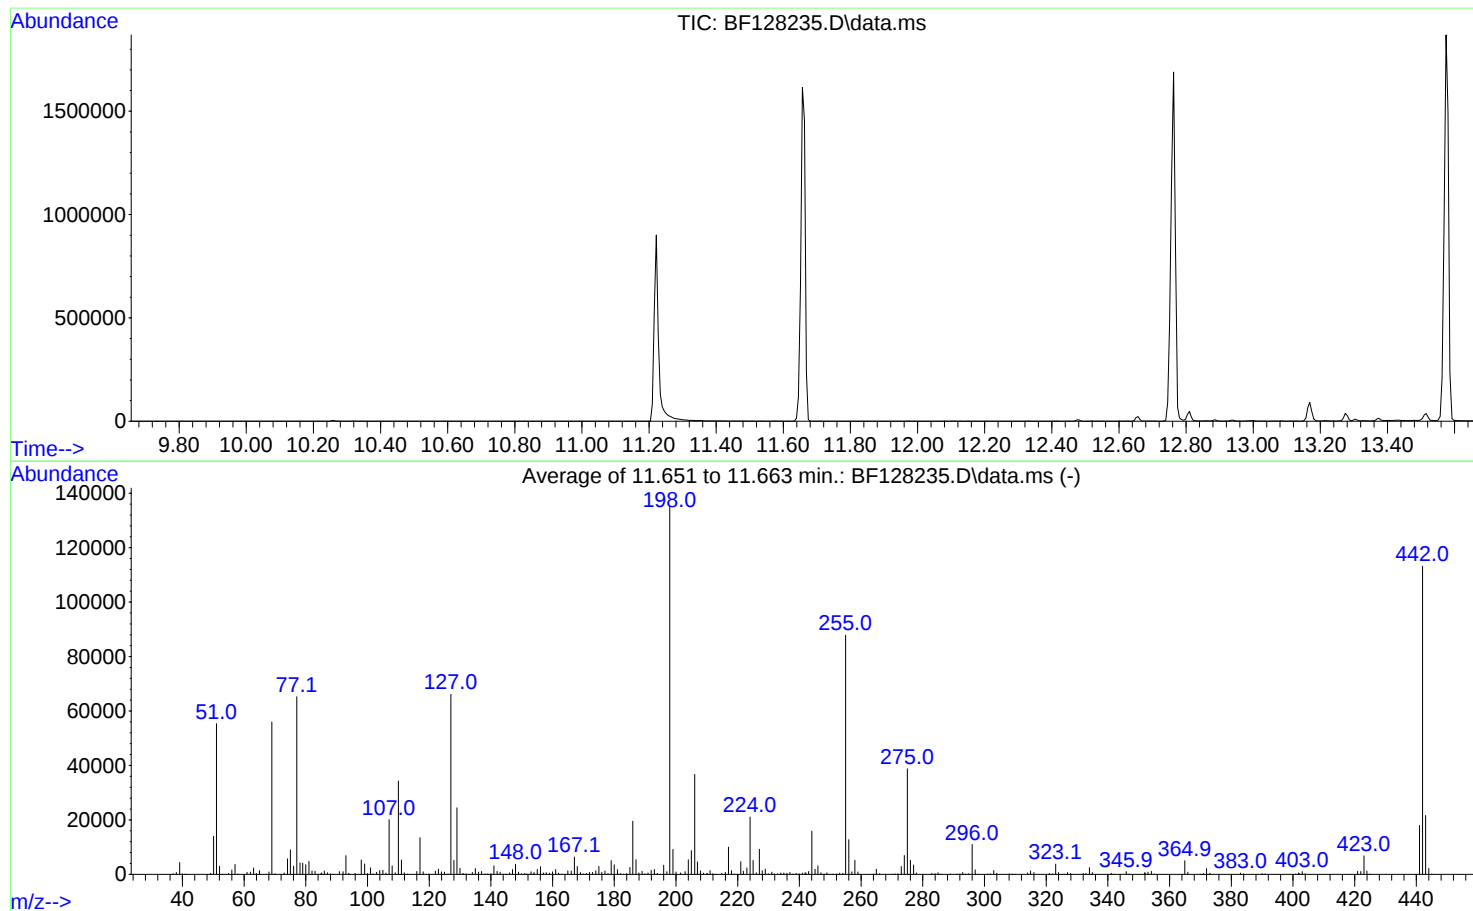




AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	55365	PASS
68	69	0.00	2	1.6	902	PASS
69	198	0.00	100	41.4	55955	PASS
70	69	0.00	2	0.4	251	PASS
127	198	10	80	48.9	66120	PASS
197	198	0.00	2	0.7	1008	PASS
198	198	100	100	100.0	135115	PASS
199	198	5	9	6.8	9170	PASS
275	198	10	60	28.7	38772	PASS
365	198	1	100	3.7	4983	PASS
441	198	0.01	100	13.3	18002	PASS
442	442	50	100	100.0	113173	PASS
443	442	15	24	19.1	21649	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
 Data File : BF128235.D
 Acq On : 13 May 2022 12:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 13 17:07:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 09 15:30:11 2022
 Response via : Initial Calibration

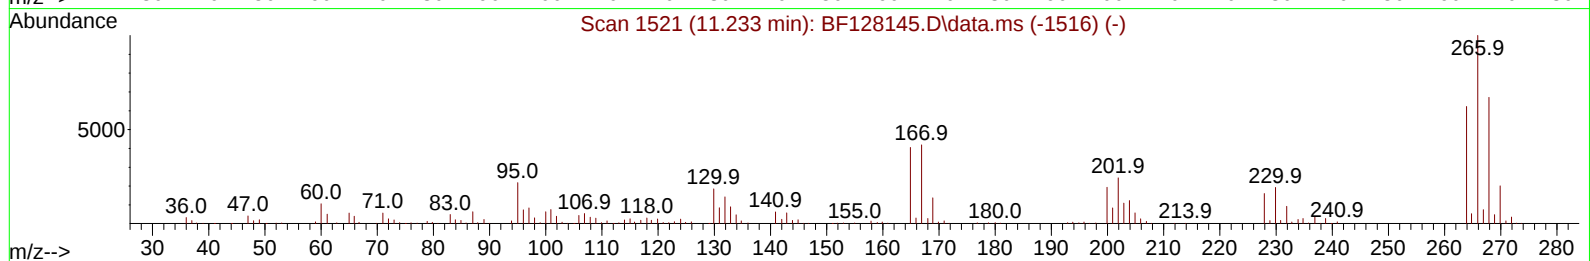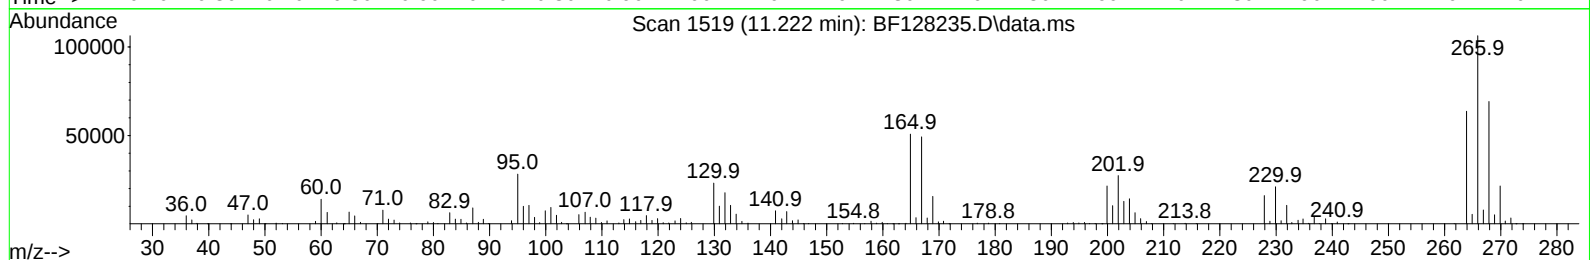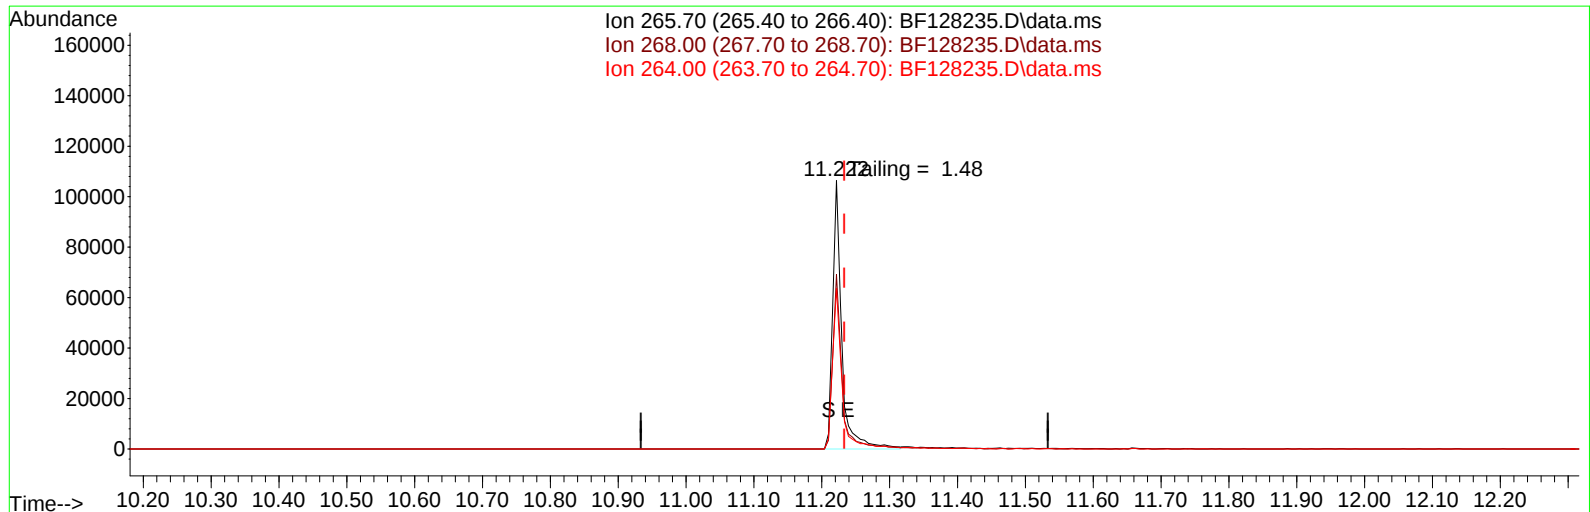

TIC: BF128235.D\data.ms

(70) Pentachlorophenol (C)

11.222min (-0.012) 29594.29 ng




response 99222

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	65.06
264.00	66.40	59.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051322\
 Data File : BF128235.D
 Acq On : 13 May 2022 12:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 13 17:07:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 09 15:30:11 2022
 Response via : Initial Calibration

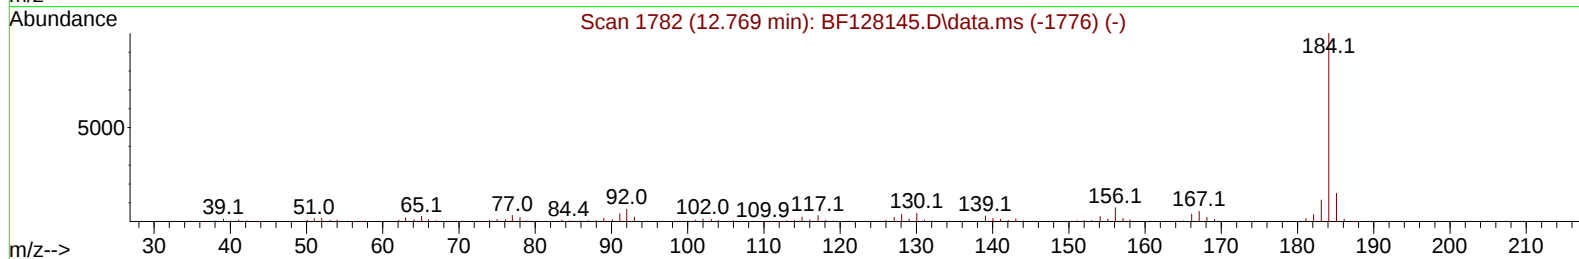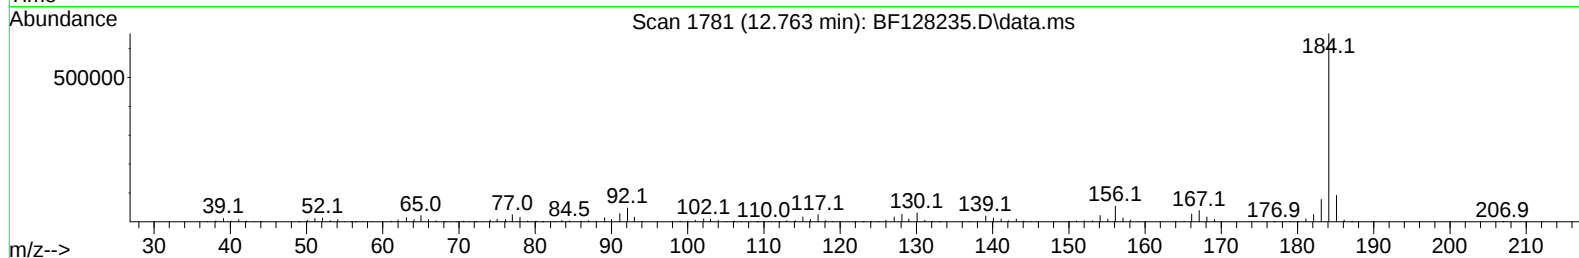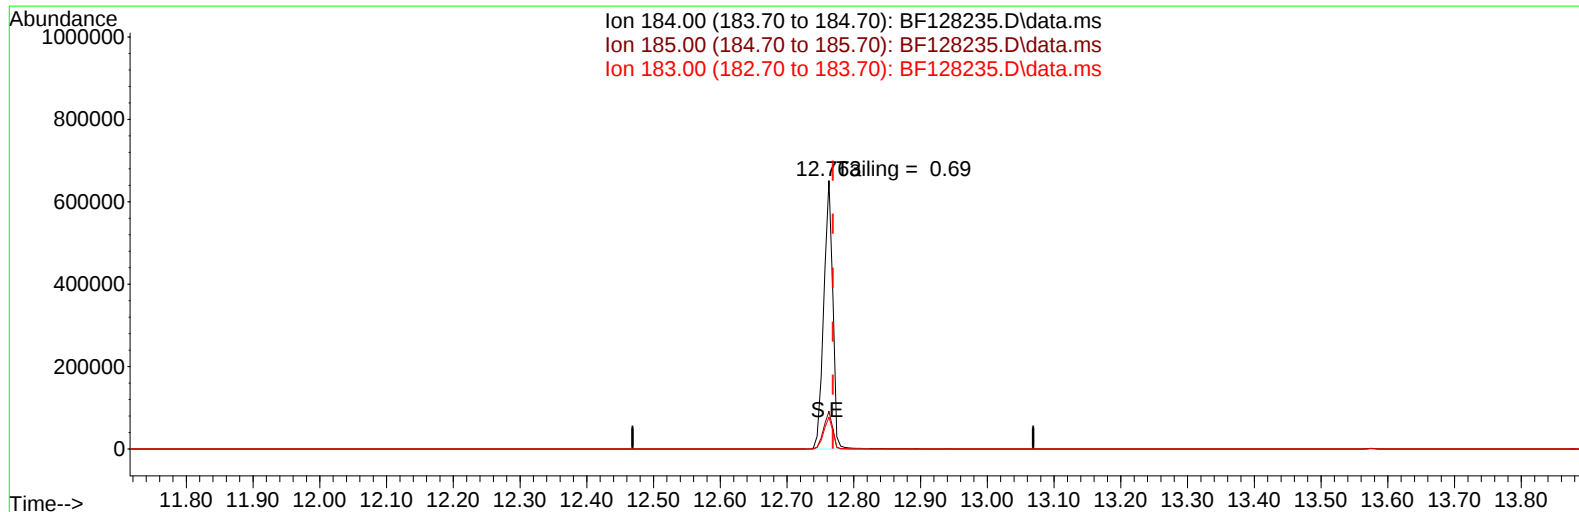

TIC: BF128235.D\data.ms

(77) Benzidine

12.763min (-0.006) 0.00 ng

response 607741

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.10
183.00	11.20	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/13/2022	BNA_F	<u>BF128235.D</u>
Compound Name	Response	Retention Time
DDT	328457	13.574
DDD	8659	13.274
DDE	1091	12.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9750	338207	2.88

Instrument :
BNA_F
ClientSampleId :
DFTPP