

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051324\
 Data File : BF137904.D
 Acq On : 13 May 2024 15:53
 Operator : CG\JU
 Sample : P2432-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-04-011

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137904.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.181	10	16	21	rVB2	39141	82534	2.47%	0.373%
2	2.393	45	52	58	rBV	1415624	1930855	57.76%	8.738%
3	5.663	603	608	611	rBV	2372283	2029054	60.69%	9.182%
4	6.651	771	776	779	rBV	2205803	2023509	60.53%	9.157%
5	7.040	838	842	845	rBV	1028479	766011	22.91%	3.466%
6	7.598	932	937	940	rBV	1590891	1312352	39.26%	5.939%
7	8.322	1056	1060	1063	rBV	1281128	1024358	30.64%	4.636%
8	9.398	1238	1243	1246	rBV	3087220	2858327	85.50%	12.935%
9	10.080	1355	1359	1363	rBV	1544894	1230573	36.81%	5.569%
10	10.163	1369	1373	1379	rVB2	33366	44526	1.33%	0.201%
11	10.875	1489	1494	1497	rBV	1786986	1662261	49.72%	7.522%
12	11.575	1609	1613	1616	rBV	1584250	1300424	38.90%	5.885%
13	12.074	1695	1698	1702	rBV	36448	39573	1.18%	0.179%
14	12.792	1816	1820	1822	rBV	44794	39213	1.17%	0.177%
15	13.021	1852	1859	1865	rVB2	58032	68355	2.04%	0.309%
16	13.163	1878	1883	1886	rBV	3875179	3343104	100.00%	15.129%
17	14.045	2027	2033	2035	rBV2	44840	41019	1.23%	0.186%
18	14.080	2035	2039	2055	rVB9	23747	78181	2.34%	0.354%
19	14.221	2059	2063	2067	rBV	1376187	1197236	35.81%	5.418%
20	15.786	2323	2329	2340	rVB	797236	1026133	30.69%	4.644%




Sum of corrected areas: 22097598

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051324\
Data File : BF137904.D
Acq On : 13 May 2024 15:53
Operator : CG\JU
Sample : P2432-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-04-011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

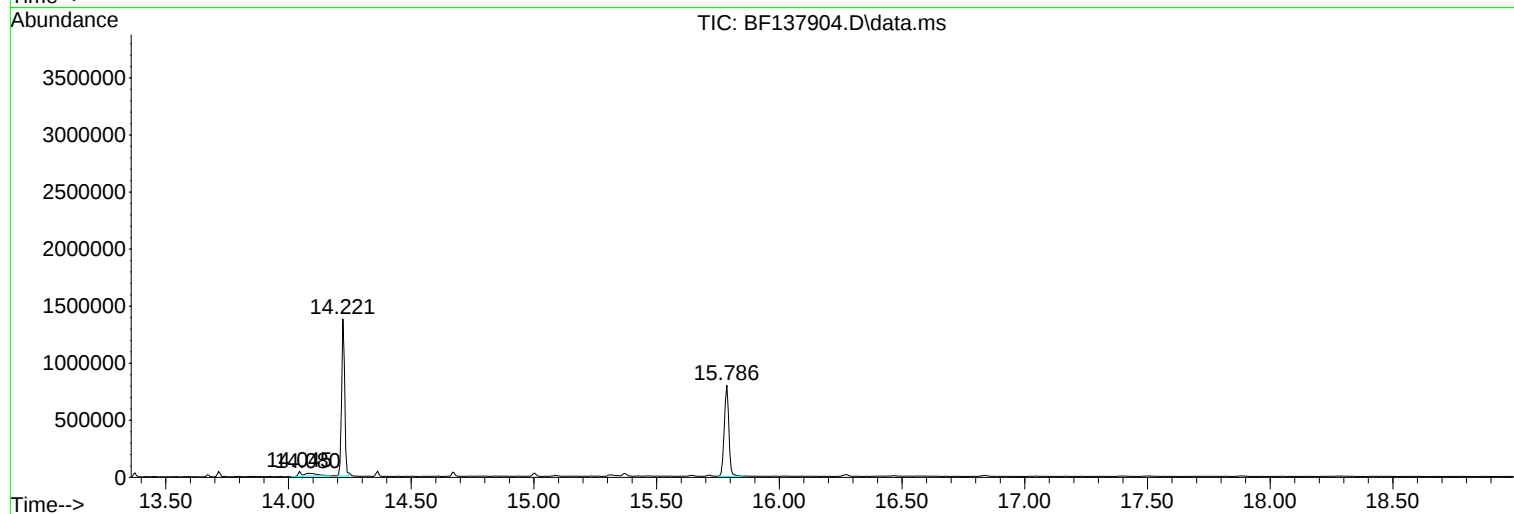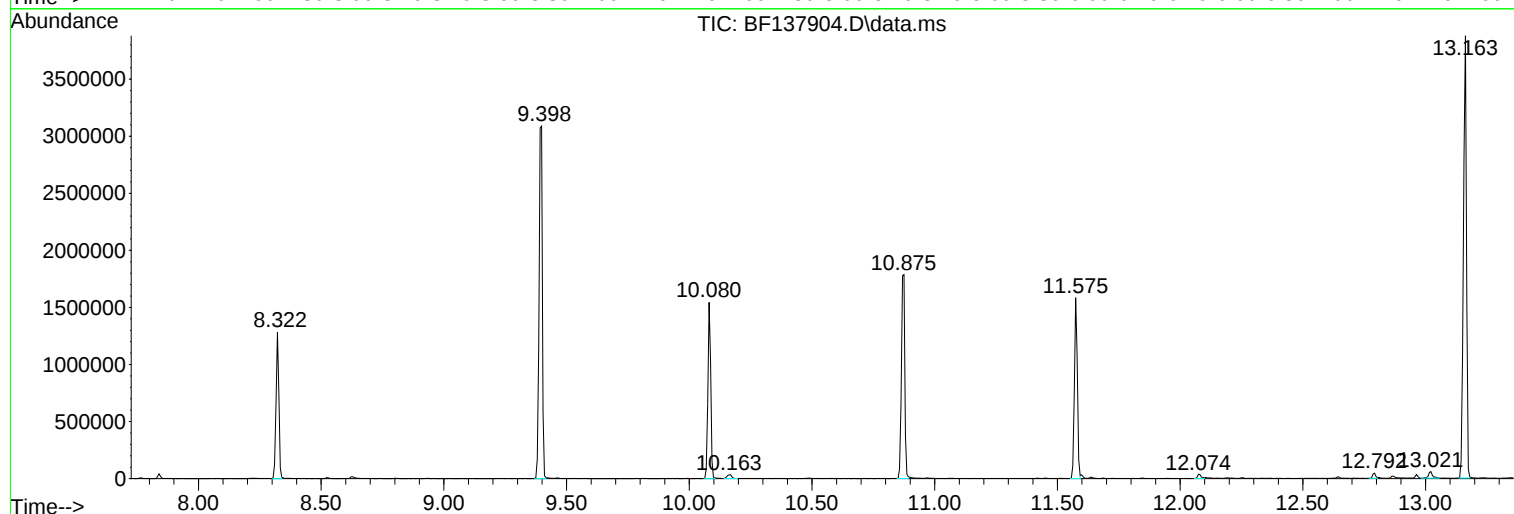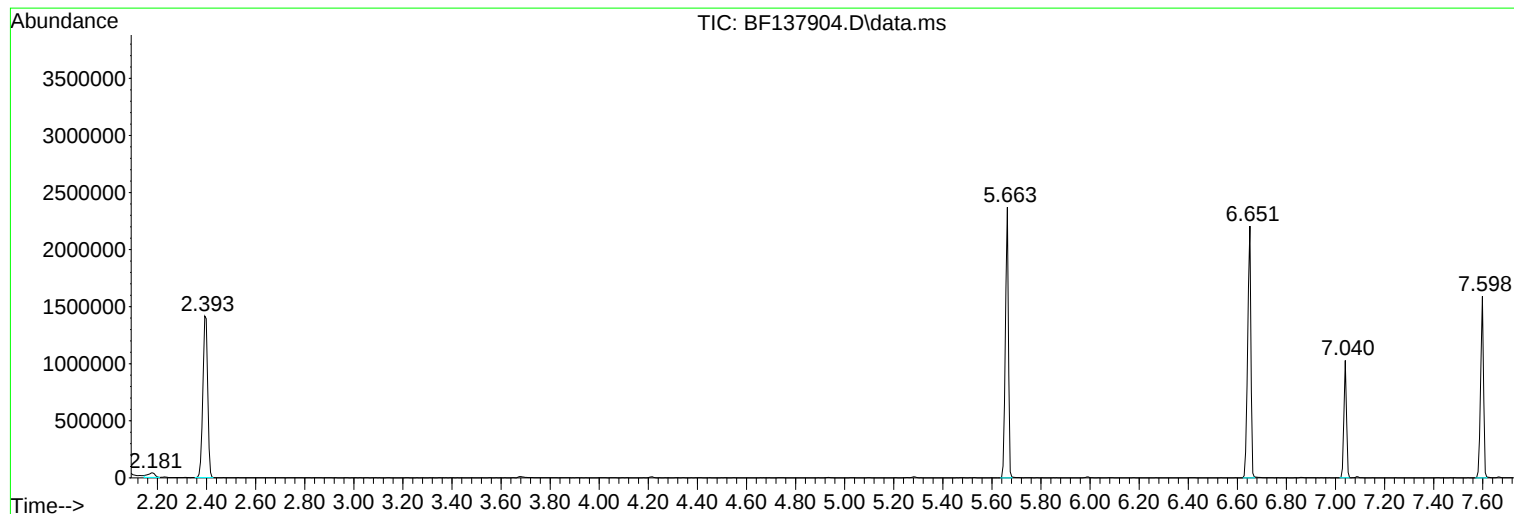

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051324\
Data File : BF137904.D
Acq On : 13 May 2024 15:53
Operator : CG\JU
Sample : P2432-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-04-011










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.393	50.41 ng	1930860	1,4-Dichlorobenzene-d4	7.040

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	22
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	17

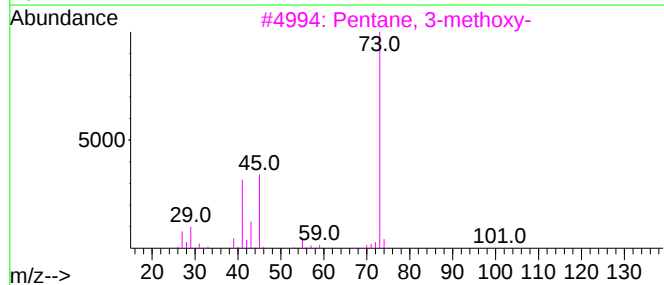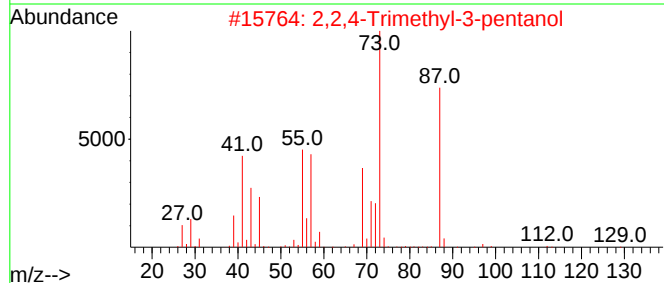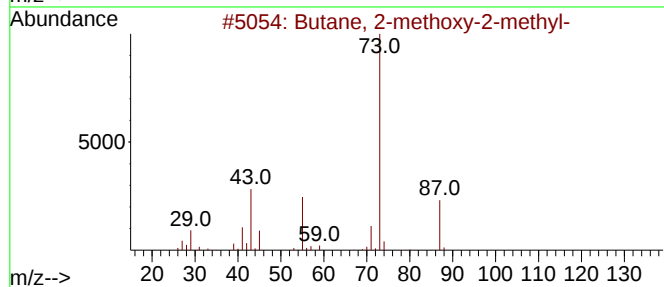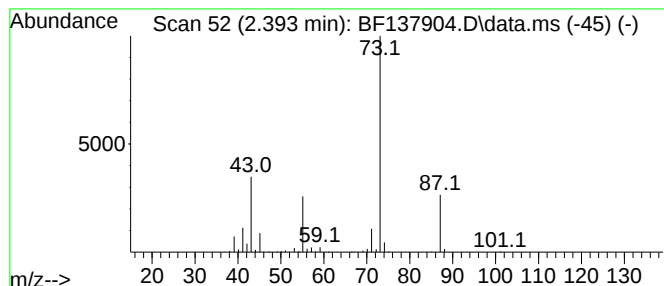

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051324\
Data File : BF137904.D
Acq On : 13 May 2024 15:53
Operator : CG\JU
Sample : P2432-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-04-011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.393	50.4	ng	1930860	1	7.040	766011	20.0