


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051324\
Data File : BF137896.D
Acq On : 13 May 2024 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

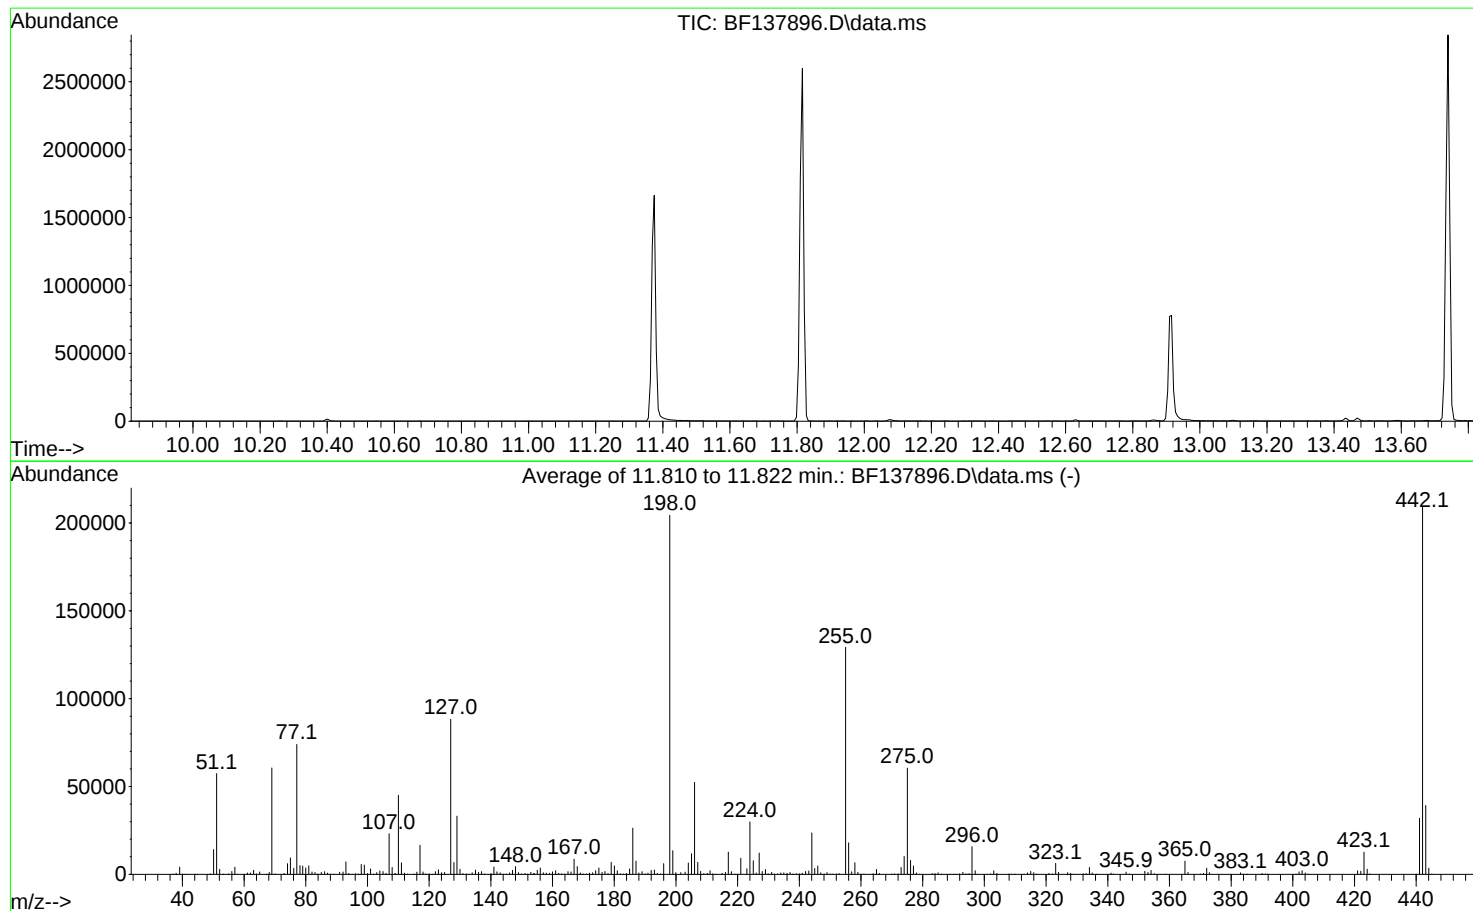

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	57427	PASS
68	69	0.00	2	1.8	1111	PASS
69	198	0.00	100	29.6	60601	PASS
70	69	0.00	2	0.5	321	PASS
127	198	10	80	43.2	88288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	204392	PASS
199	198	5	9	6.6	13447	PASS
275	198	10	60	29.6	60456	PASS
365	198	1	100	3.7	7536	PASS
441	198	0.01	100	15.6	31859	PASS
442	442	50	100	100.0	209403	PASS
443	442	15	24	18.8	39275	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/13/2024	BNA_F	<u>BF137896.D</u>
Compound Name	Response	Retention Time
DDT	454467	13.739
DDD	7301	13.433
DDE	825	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8126	462593	1.76

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051324\
Data File : BF137896.D
Acq On : 13 May 2024 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 13 13:26:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

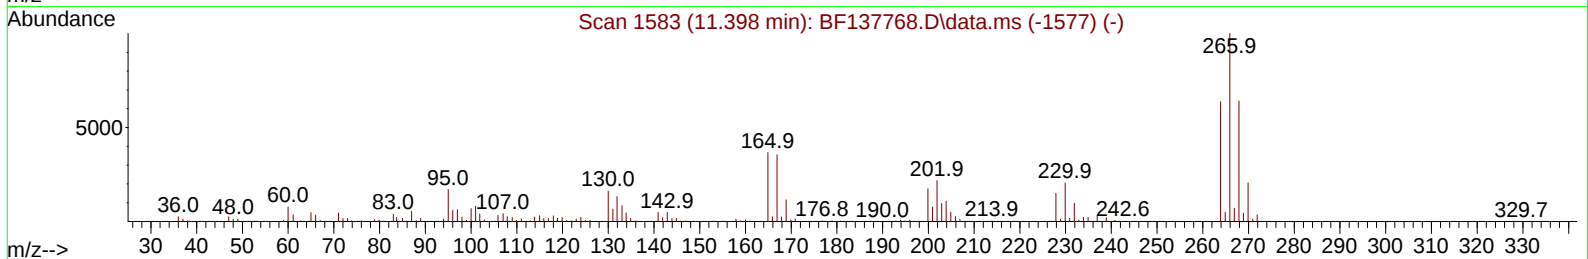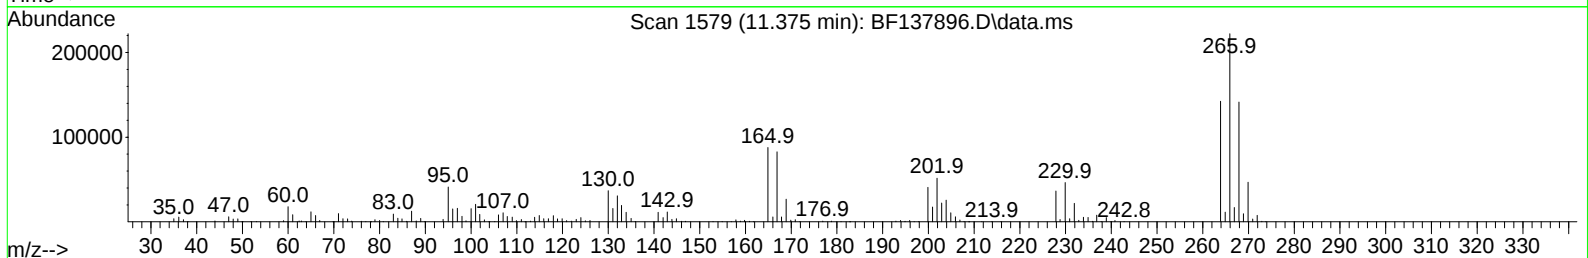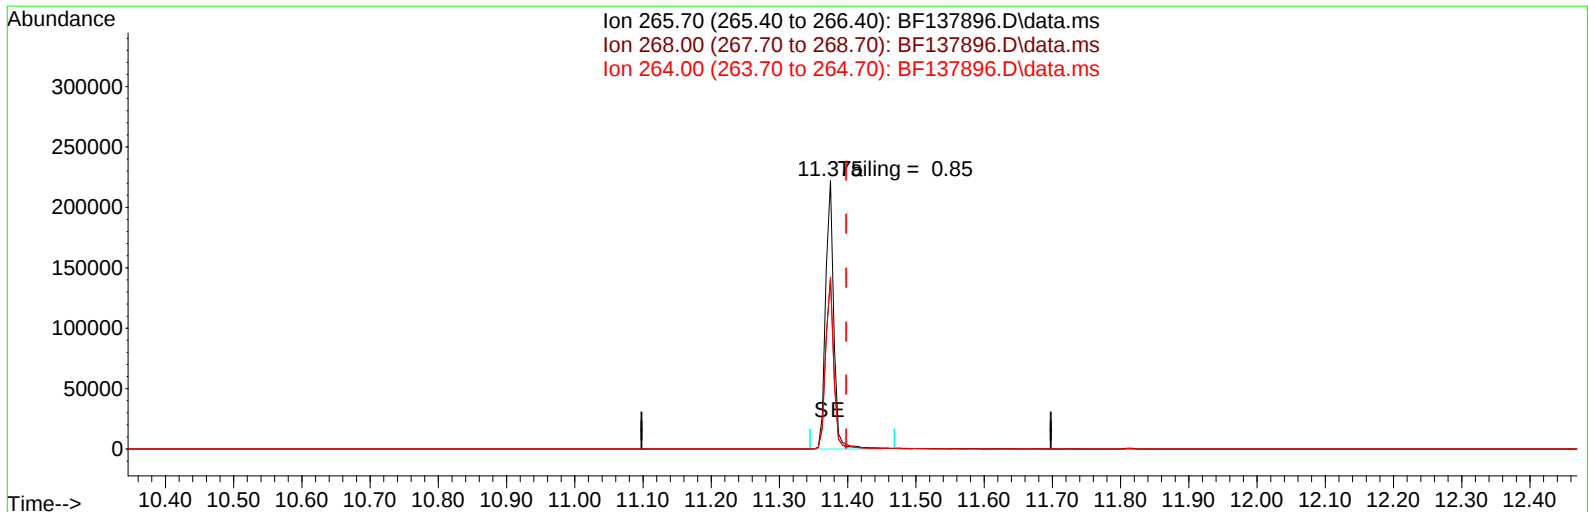

TIC: BF137896.D\data.ms

(70) Pentachlorophenol (C)

11.375min (-0.023) 24375.43 ng




response 184173

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	63.70
264.00	63.70	64.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051324\
Data File : BF137896.D
Acq On : 13 May 2024 11:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 13 13:26:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

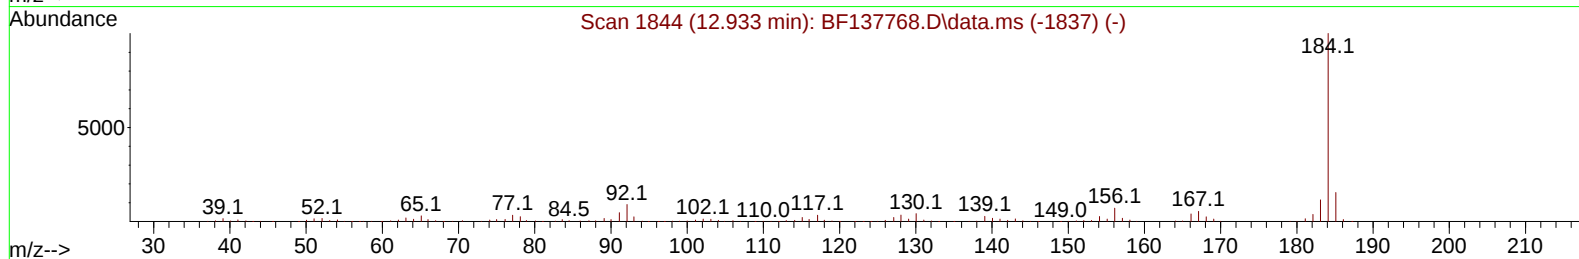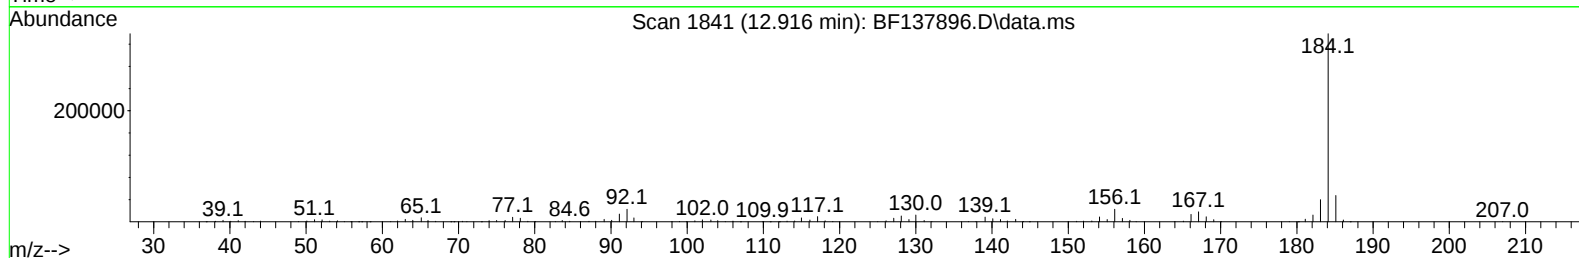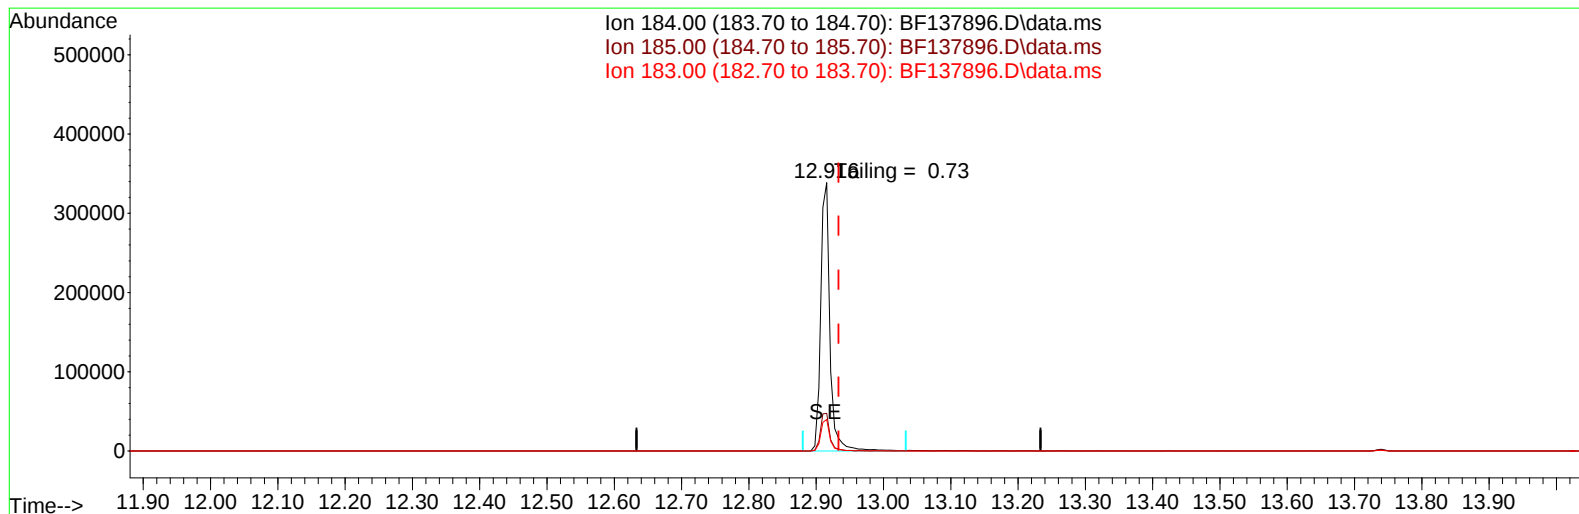

TIC: BF137896.D\data.ms

(77) Benzidine

12.916min (-0.018) 0.00 ng

response 324150

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.02
183.00	11.50	11.77
0.00	0.00	0.00