

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051325\
 Data File : BF142337.D
 Acq On : 13 May 2025 11:17
 Operator : RC/JU
 Sample : PB167951BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB167951BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.275	4	14	20	rVB	51019	94935	1.22%	0.205%
2	5.145	495	502	514	rBV	380670	623935	8.04%	1.346%
3	5.528	560	567	572	rBV	4050179	5823711	75.03%	12.561%
4	6.522	729	736	742	rBV	3808375	5805875	74.80%	12.523%
5	6.904	796	801	806	rBV	1117548	1360933	17.53%	2.935%
6	7.463	889	896	901	rBV	2747531	3840898	49.49%	8.284%
7	8.186	1012	1019	1024	rBV	1376793	1817846	23.42%	3.921%
8	9.263	1195	1202	1207	rBV	5237757	7223983	93.07%	15.581%
9	9.939	1311	1317	1322	rBV	1695886	2113366	27.23%	4.558%
10	10.727	1445	1451	1467	rBV	3457380	4655753	59.98%	10.042%
11	11.427	1564	1570	1575	rBV	1821080	2248640	28.97%	4.850%
12	13.016	1834	1840	1846	rBV	5558315	7761569	100.00%	16.741%
13	14.068	2013	2019	2028	rBV	1345321	1768081	22.78%	3.814%
14	15.557	2266	2272	2290	rBV	779521	1223930	15.77%	2.640%




Sum of corrected areas: 46363455

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051325\
Data File : BF142337.D
Acq On : 13 May 2025 11:17
Operator : RC/JU
Sample : PB167951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167951BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

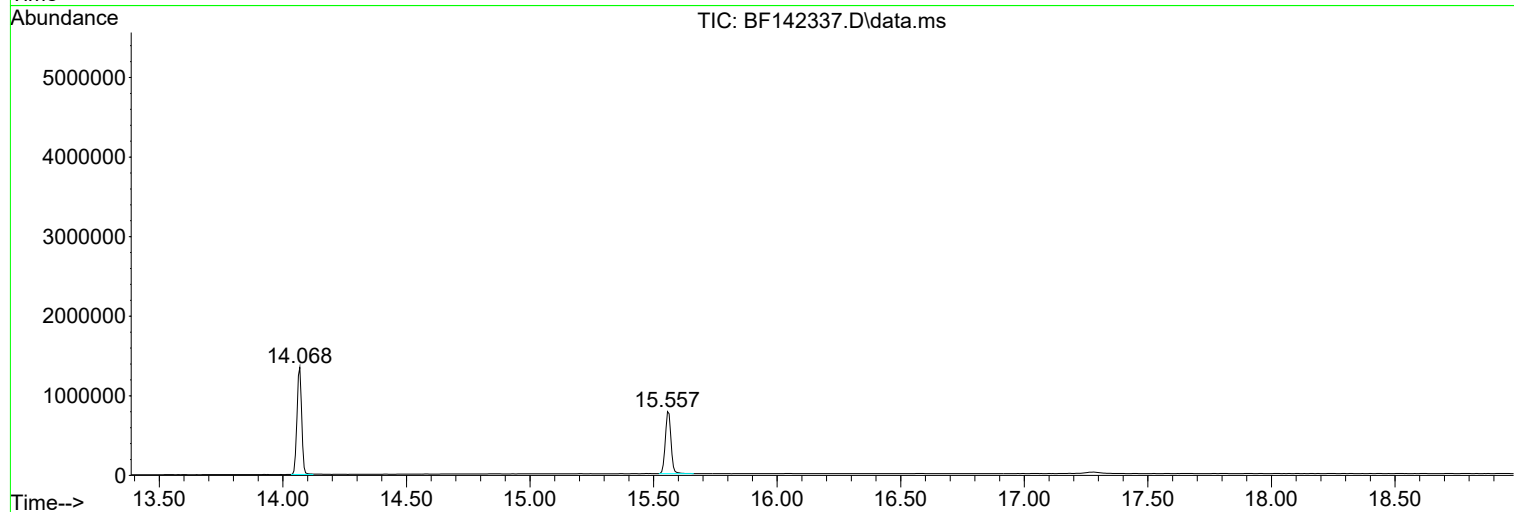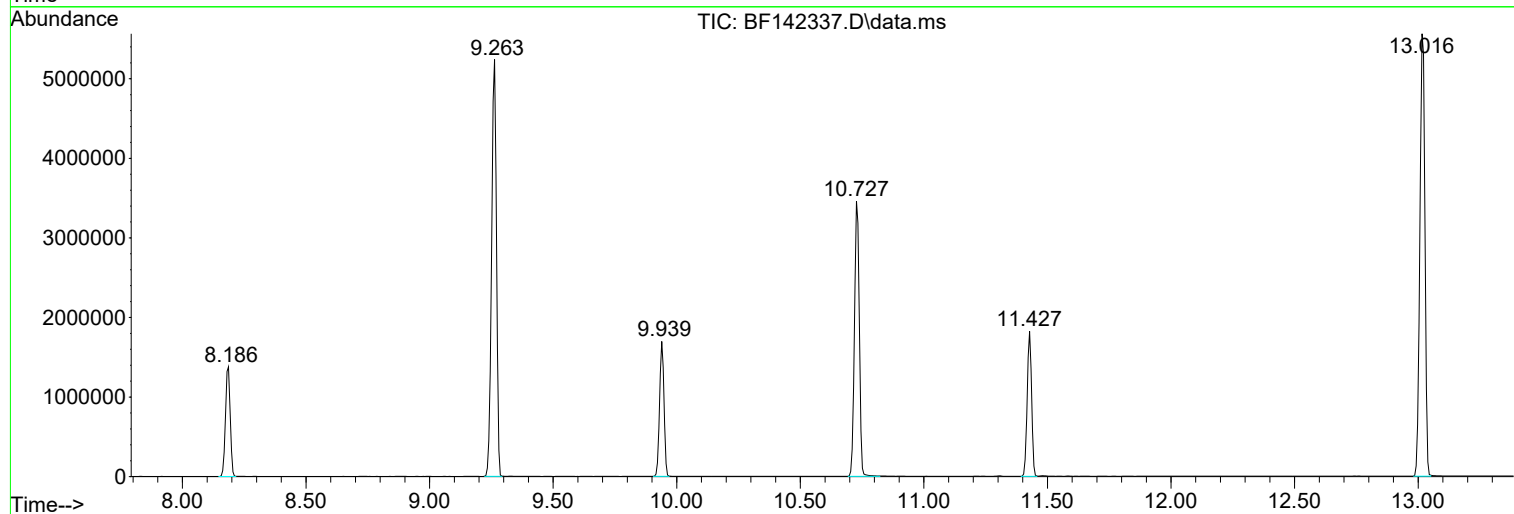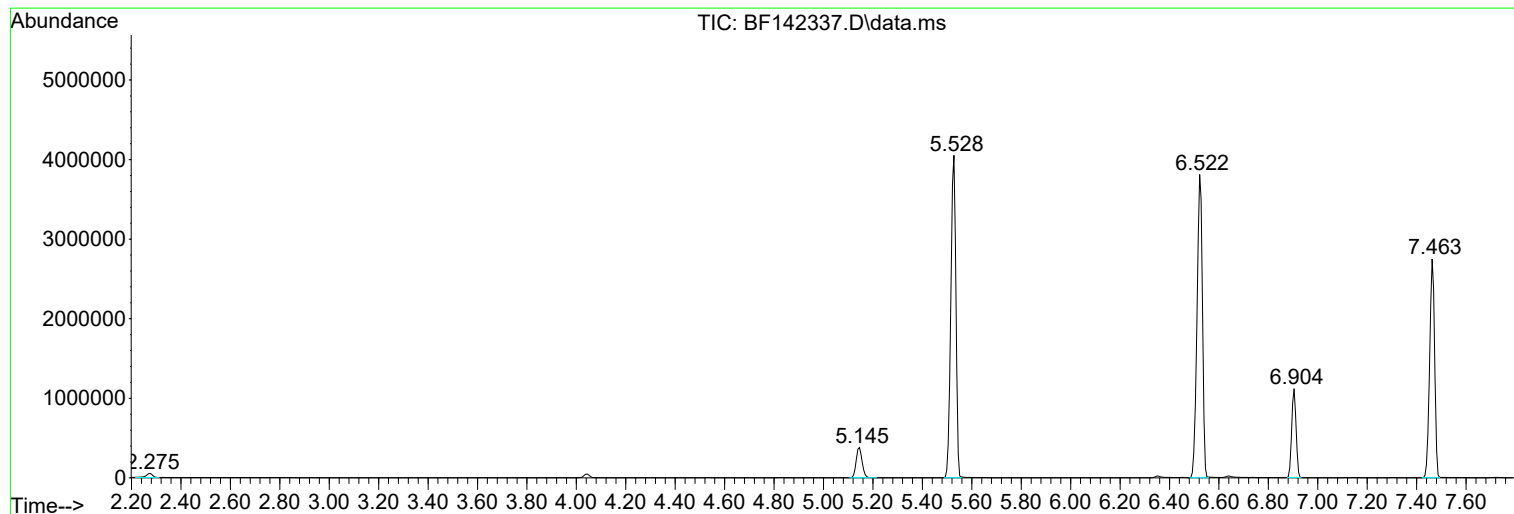

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051325\
Data File : BF142337.D
Acq On : 13 May 2025 11:17
Operator : RC/JU
Sample : PB167951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB167951BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.145	9.17 ng	623935	1,4-Dichlorobenzene-d4	6.904	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	83
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	36
3	Acetone	58	C3H6O	000067-64-1	16
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	12
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12

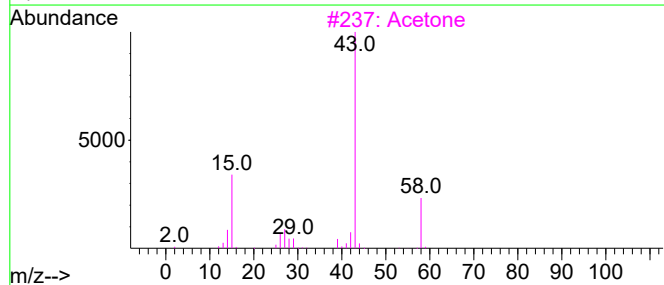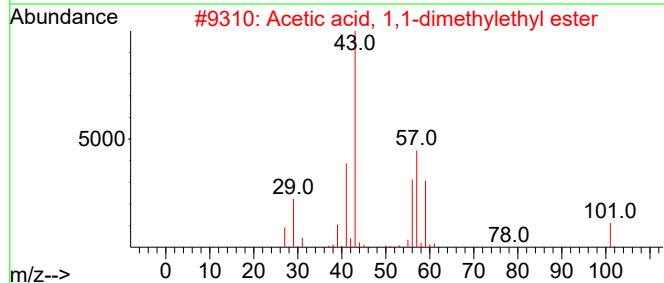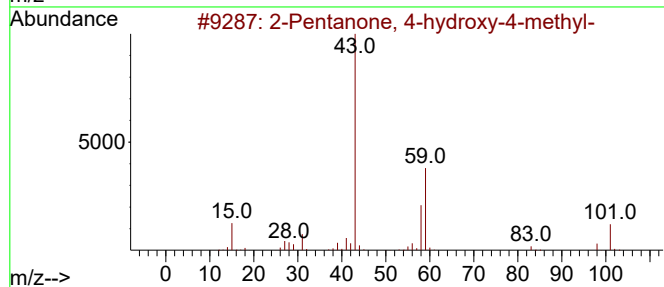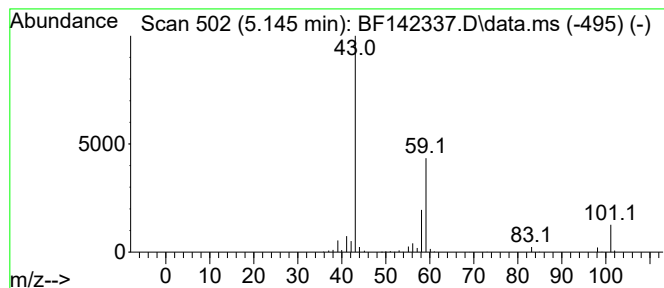

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051325\
Data File : BF142337.D
Acq On : 13 May 2025 11:17
Operator : RC/JU
Sample : PB167951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167951BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.145	9.2	ng	623935	1	6.904	1360930	20.0