


Data Path : Z:\HPCHEM1\BNA_F\Data\BF051415\
 Data File : BF079235.D
 Acq On : 14 May 2015 14:13
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 14 16:56:55 2015

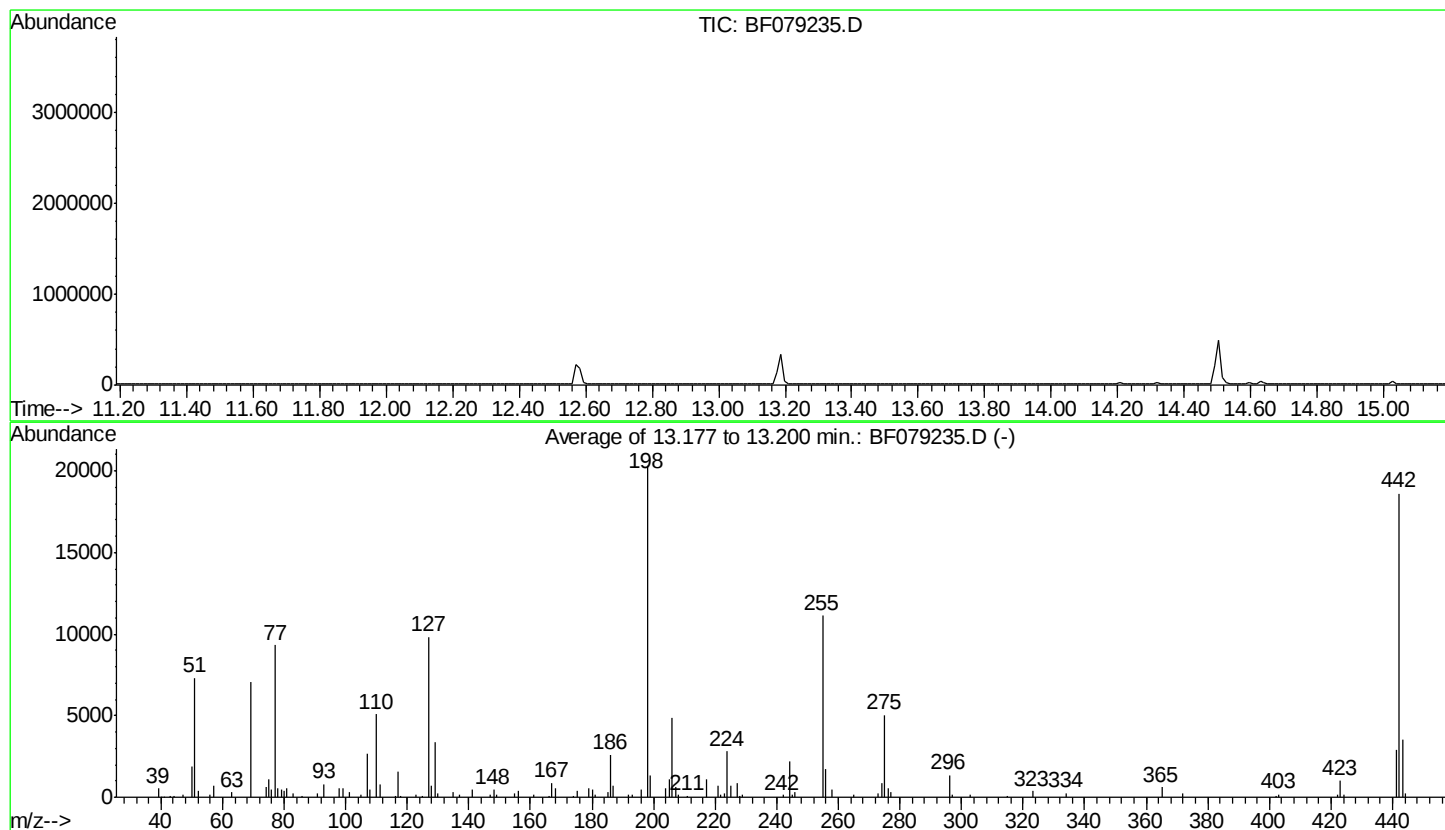

AutoFind: Scans 1049, 1050, 1051; Background Corrected with Scan 1046

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	7307	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.6	7042	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.4	9844	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20329	PASS
199	198	5	9	6.5	1318	PASS
275	198	10	60	24.9	5061	PASS
365	198	1	100	3.0	614	PASS
441	442	0.01	24	15.5	2893	PASS
442	198	50	100	91.7	18639	PASS
443	442	15	24	19.2	3571	PASS