


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051415\
 Data File : BF079255.D
 Acq On : 15 May 2015 4:06
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 15 02:17:41 2015

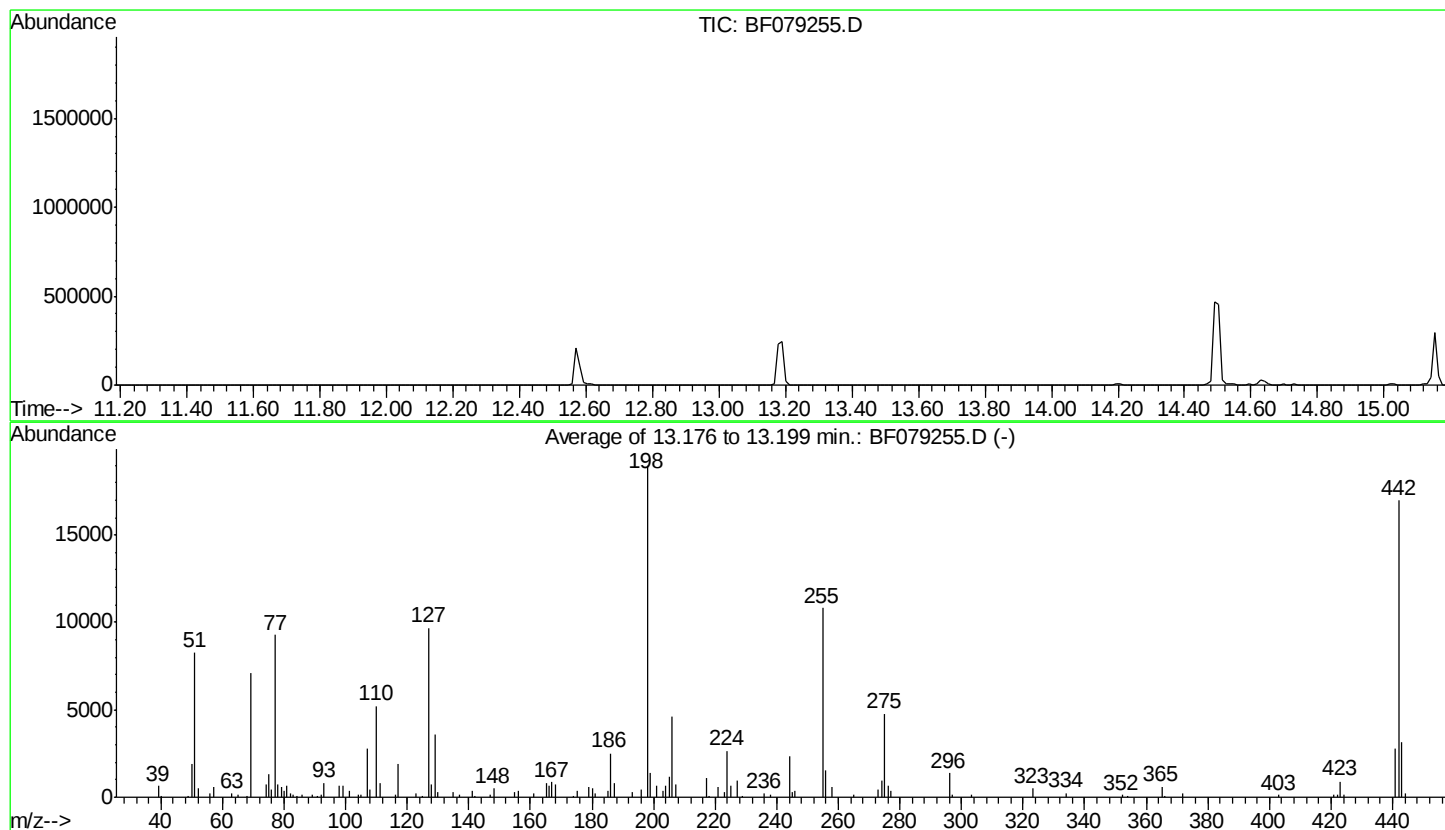

AutoFind: Scans 1049, 1050, 1051; Background Corrected with Scan 1045

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	8241	PASS
68	69	0.00	2	1.5	104	PASS
69	198	0.00	100	37.3	7076	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.0	9668	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18968	PASS
199	198	5	9	7.4	1405	PASS
275	198	10	60	25.3	4797	PASS
365	198	1	100	3.2	615	PASS
441	442	0.01	24	16.6	2817	PASS
442	198	50	100	89.4	16963	PASS
443	442	15	24	18.8	3186	PASS