
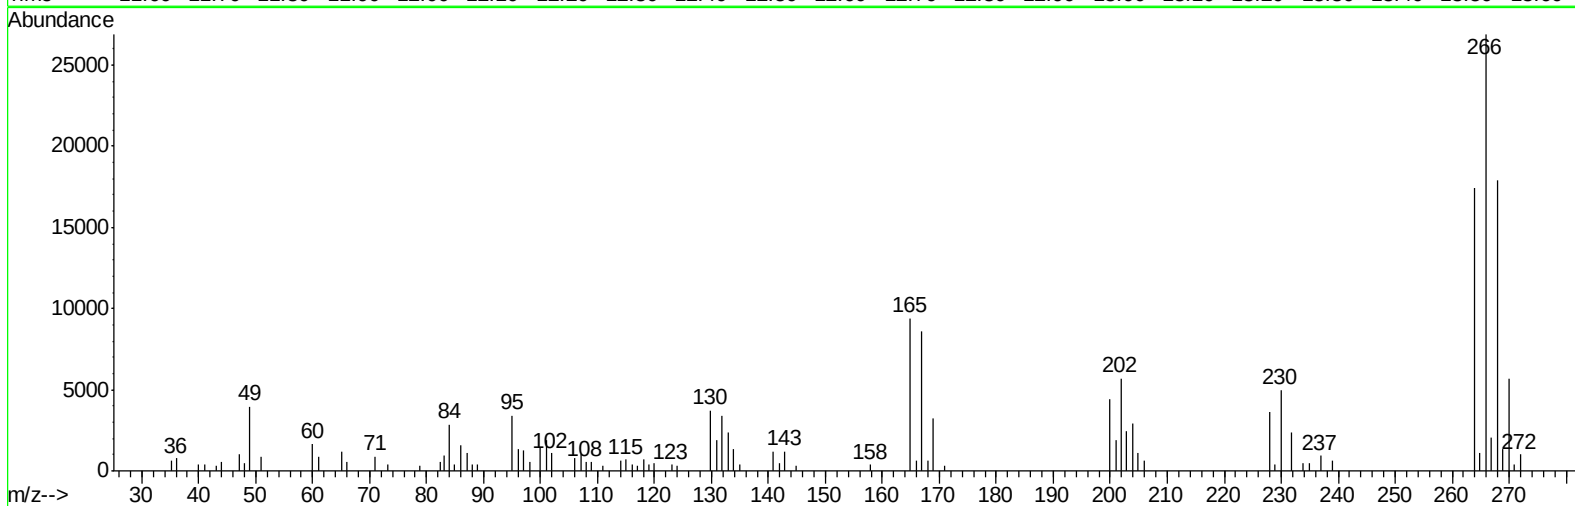


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051415\
Data File : BF079235.D
Acq On : 14 May 2015 14:13
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 07:07:09 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 15 06:46:28 2015
Response via : Initial Calibration

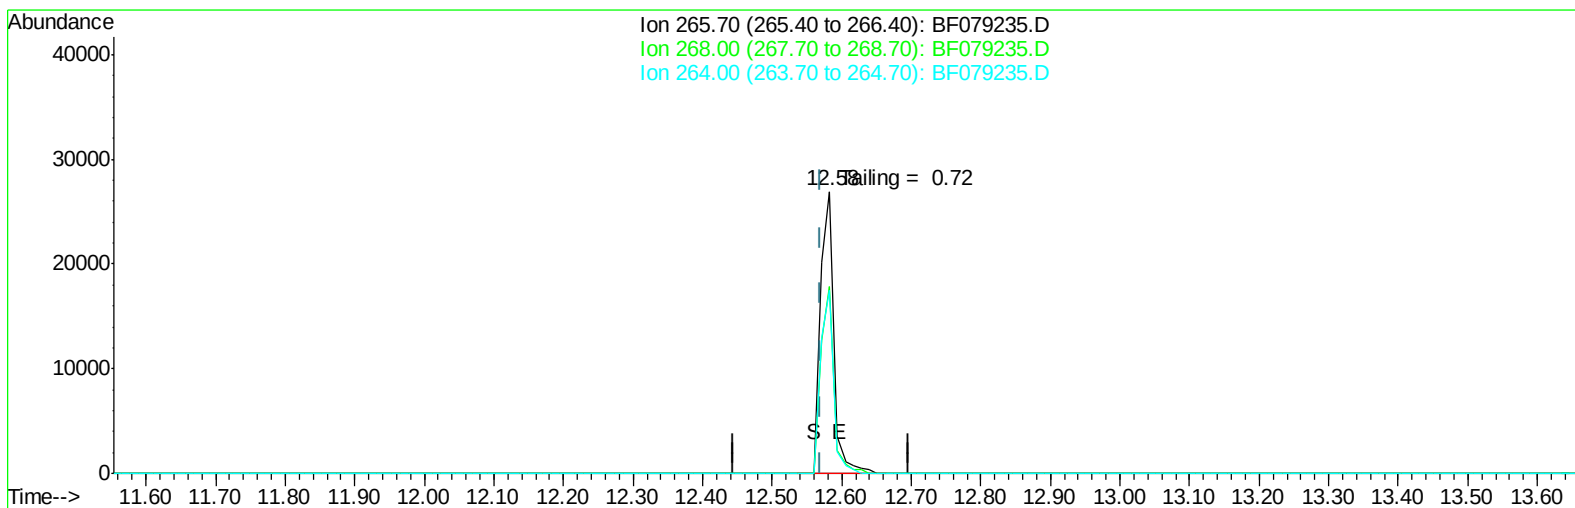

TIC: BF079235.D

(69) Pentachlorophenol (C)



12.582min (+0.012) 15441.25ng

response 36469

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.60
264.00	63.60	64.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051415\
Data File : BF079235.D
Acq On : 14 May 2015 14:13
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 07:07:09 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 15 06:46:28 2015
Response via : Initial Calibration

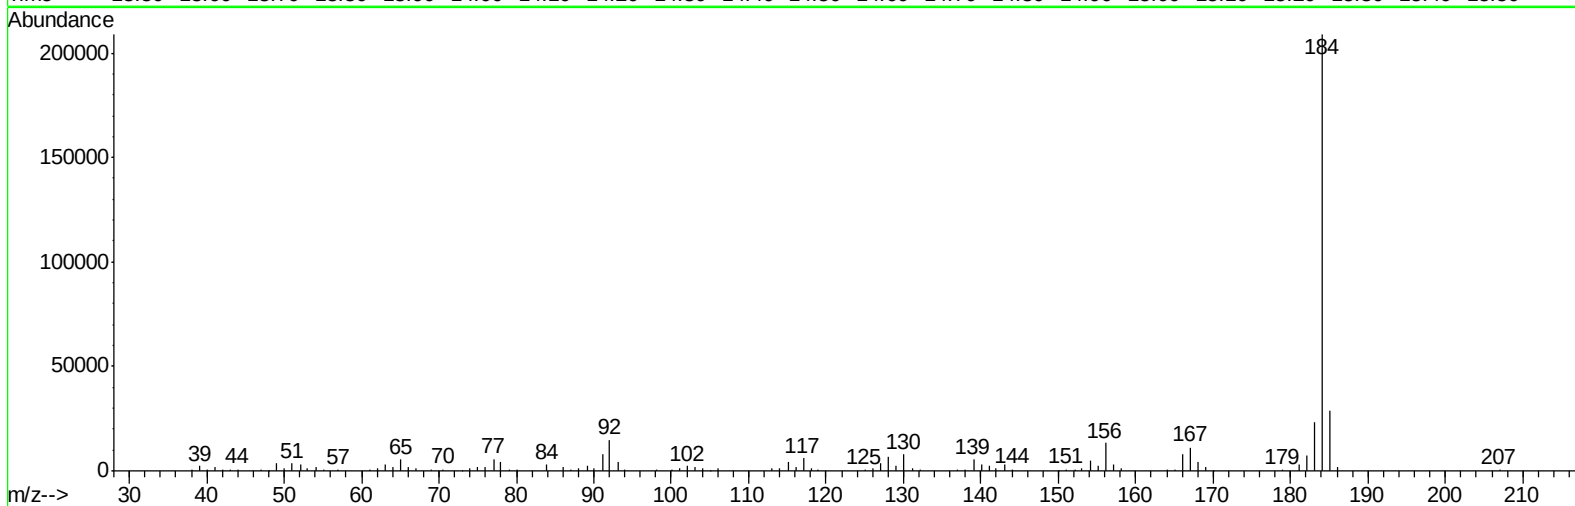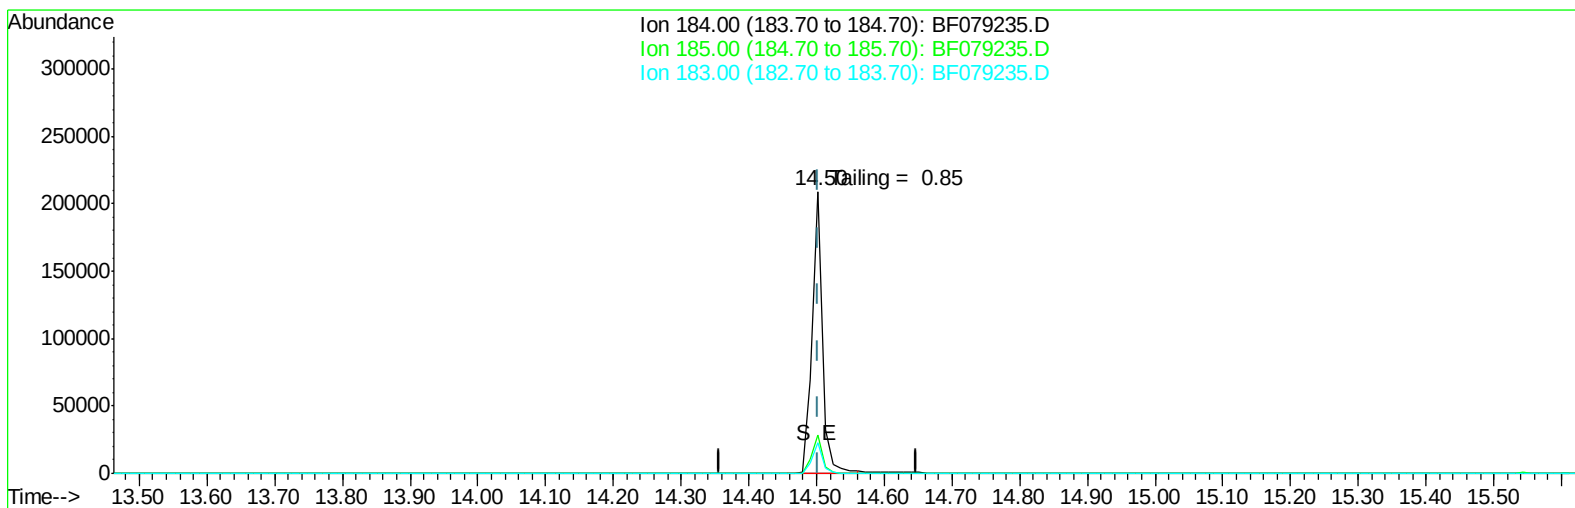

TIC: BF079235.D

(76) Benzidine

14.503min (+0.000) 10315.35ng

response 227411

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	13.87
183.00	11.20	11.07
0.00	0.00	0.00