

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051415\
 Data File : BF079248.D
 Acq On : 14 May 2015 23:12
 Operator : TP/IZ
 Sample : G2201-03DL 25X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SUMP1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.484	24	26	39	rVB	129336	329010	4.43%	0.237%
2	1.815	53	55	93	rVB	2501415	4815369	64.89%	3.472%
3	7.622	561	563	564	rBV2	255426	312933	4.22%	0.226%
4	7.885	583	586	587	rBV	333601	367465	4.95%	0.265%
5	7.976	592	594	597	rBV	1176545	1038610	14.00%	0.749%
6	8.170	608	611	613	rBV	322341	384647	5.18%	0.277%
7	8.205	613	614	618	rVB	871998	767941	10.35%	0.554%
8	8.353	622	627	628	rBV4	413302	930298	12.54%	0.671%
9	8.388	628	630	632	rBV2	400851	565594	7.62%	0.408%
10	8.433	632	634	636	rVB2	345020	507583	6.84%	0.366%
11	8.479	636	638	640	rVB2	1008868	1271966	17.14%	0.917%
12	8.525	640	642	645	rVB2	868478	1079900	14.55%	0.779%
13	8.570	645	646	647	rBV	747058	776556	10.46%	0.560%
14	8.593	647	648	650	rVB	558007	648902	8.74%	0.468%
15	8.650	650	653	654	rBV	330443	357345	4.82%	0.258%
16	8.810	658	667	668	rBV2	2753426	5090365	68.59%	3.670%
17	8.902	674	675	679	rBV2	716531	1280231	17.25%	0.923%
18	9.039	682	687	691	rBV6	676649	1649294	22.22%	1.189%
19	9.108	691	693	694	rBV	312734	340111	4.58%	0.245%
20	9.176	694	699	700	rBV4	520365	1340027	18.06%	0.966%
21	9.222	702	703	704	rVB	532380	365213	4.92%	0.263%
22	9.256	704	706	707	rBV	947375	840710	11.33%	0.606%
23	9.302	707	710	713	rVB3	908508	1596291	21.51%	1.151%
24	9.359	713	715	719	rBV3	1309110	2359908	31.80%	1.702%
25	9.428	719	721	724	rBV2	1730548	1824262	24.58%	1.315%
26	9.576	731	734	736	rBV	2740872	3962301	53.39%	2.857%
27	9.622	736	738	740	rVB	1022202	1017494	13.71%	0.734%
28	9.679	740	743	745	rVB2	1051874	1820722	24.53%	1.313%
29	9.736	745	748	749	rBV2	168158	316929	4.27%	0.229%
30	9.805	752	754	755	rBV2	611891	912667	12.30%	0.658%
31	9.828	755	756	758	rVB2	1542157	1216145	16.39%	0.877%
32	9.919	761	764	765	rBV3	645901	1214120	16.36%	0.875%
33	9.942	765	766	767	rVB	646232	442992	5.97%	0.319%
34	9.976	767	769	772	rVB3	597831	971619	13.09%	0.701%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051415\
 Data File : BF079248.D
 Acq On : 14 May 2015 23:12
 Operator : TP/IZ
 Sample : G2201-03DL 25X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SUMP1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.022	772	773	775	rVB	1119946	935444	12.61%	0.674%
36	10.068	775	777	778	rBV2	820314	1114488	15.02%	0.804%
37	10.102	778	780	783	rVB	1732370	2015679	27.16%	1.453%
38	10.171	783	786	789	rBV4	393230	874215	11.78%	0.630%
39	10.228	789	791	792	rBV2	197777	303036	4.08%	0.219%
40	10.273	792	795	797	rBV	3324673	4427098	59.66%	3.192%
41	10.331	797	800	801	rVB	1242789	1254820	16.91%	0.905%
42	10.365	801	803	805	rVB2	498887	649835	8.76%	0.469%
43	10.456	810	811	814	rBV2	962749	1697243	22.87%	1.224%
44	10.559	816	820	821	rBV2	890075	1449765	19.54%	1.045%
45	10.593	821	823	824	rVB2	891181	1201506	16.19%	0.866%
46	10.674	826	830	831	rBV4	1796344	2697194	36.34%	1.945%
47	10.799	840	841	843	rBV2	484657	413701	5.57%	0.298%
48	10.936	850	853	855	rVV	3837686	4655801	62.74%	3.357%
49	10.971	855	856	858	rVB2	931374	1020233	13.75%	0.736%
50	11.108	867	868	871	rVB	581343	899925	12.13%	0.649%
51	11.234	874	879	880	rBV3	1372417	2901606	39.10%	2.092%
52	11.291	882	884	886	rVV2	864817	1177855	15.87%	0.849%
53	11.336	886	888	890	rVB2	1527607	1744603	23.51%	1.258%
54	11.382	890	892	893	rBV	1088462	1420624	19.14%	1.024%
55	11.416	893	895	896	rVB2	682944	928994	12.52%	0.670%
56	11.485	899	901	903	rVB	515582	566559	7.63%	0.409%
57	11.565	906	908	910	rVV	4314821	4594011	61.90%	3.312%
58	11.599	910	911	914	rVB2	379587	679898	9.16%	0.490%
59	11.691	917	919	921	rBV3	513198	995077	13.41%	0.717%
60	11.736	921	923	924	rVB2	451459	415941	5.60%	0.300%
61	11.828	928	931	936	rBV	1849218	4388754	59.14%	3.164%
62	11.896	936	937	939	rVB	557408	424333	5.72%	0.306%
63	11.931	939	940	942	rBV2	771647	1020186	13.75%	0.736%
64	11.965	942	943	946	rVB2	809560	1083227	14.60%	0.781%
65	12.011	946	947	948	rBV	352211	345918	4.66%	0.249%
66	12.079	951	953	954	rBV2	302736	304473	4.10%	0.220%
67	12.114	954	956	957	rBV2	234503	349643	4.71%	0.252%
68	12.159	957	960	964	rBV	3792642	7421157	100.00%	5.351%
69	12.388	977	980	982	rBV2	1070232	2162975	29.15%	1.560%
70	12.434	982	984	986	rVV2	889077	1096481	14.78%	0.791%
71	12.468	986	987	989	rVV2	512881	560073	7.55%	0.404%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051415\
 Data File : BF079248.D
 Acq On : 14 May 2015 23:12
 Operator : TP/IZ
 Sample : G2201-03DL 25X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SUMP1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.502	989	990	993	rVV2	757070	1150794	15.51%	0.830%
73	12.559	993	995	996	rVV2	604785	807359	10.88%	0.582%
74	12.594	996	998	1001	rVB4	241946	401580	5.41%	0.290%
75	12.674	1003	1005	1006	rVV2	437575	483757	6.52%	0.349%
76	12.708	1006	1008	1010	rVV	3637729	4868807	65.61%	3.511%
77	12.742	1010	1011	1014	rVB	2323966	2674603	36.04%	1.929%
78	12.822	1015	1018	1019	rBV2	488397	794062	10.70%	0.573%
79	12.879	1021	1023	1025	rBV	423785	535072	7.21%	0.386%
80	12.925	1025	1027	1030	rBV	419614	908634	12.24%	0.655%
81	13.051	1036	1038	1040	rVB2	424946	520390	7.01%	0.375%
82	13.085	1040	1041	1043	rBV	475446	573021	7.72%	0.413%
83	13.177	1047	1049	1051	rVB	674175	777777	10.48%	0.561%
84	13.245	1052	1055	1058	rBV	3933941	4357941	58.72%	3.142%
85	13.439	1069	1072	1074	rBV2	491302	1018490	13.72%	0.734%
86	13.565	1081	1083	1085	rBV2	495921	620008	8.35%	0.447%
87	13.611	1085	1087	1089	rBV	431061	523087	7.05%	0.377%
88	13.748	1097	1099	1102	rBV	3180683	3570000	48.11%	2.574%
89	13.817	1104	1105	1107	rBV2	239013	331069	4.46%	0.239%
90	13.942	1111	1116	1119	rBV3	311915	731290	9.85%	0.527%
91	14.102	1128	1130	1131	rBV	342109	458110	6.17%	0.330%
92	14.171	1134	1136	1138	rVB	281447	338616	4.56%	0.244%
93	14.240	1140	1142	1144	rVV	2500420	2883298	38.85%	2.079%
94	14.411	1155	1157	1161	rBV2	217868	448422	6.04%	0.323%
95	14.697	1180	1182	1184	rBV	2177650	2302660	31.03%	1.660%
96	15.143	1219	1221	1223	rVB	1477298	1387555	18.70%	1.000%
97	15.577	1256	1259	1261	rBV	504738	694195	9.35%	0.501%
98	15.988	1293	1295	1302	rVB	315746	413515	5.57%	0.298%
99	16.103	1302	1305	1307	rVV	426717	610917	8.23%	0.440%
100	17.828	1453	1456	1459	rBV	515371	594531	8.01%	0.429%


Sum of corrected areas: 138687451

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051415\
Data File : BF079248.D
Acq On : 14 May 2015 23:12
Operator : TP/IZ
Sample : G2201-03DL 25X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SUMP1DL

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

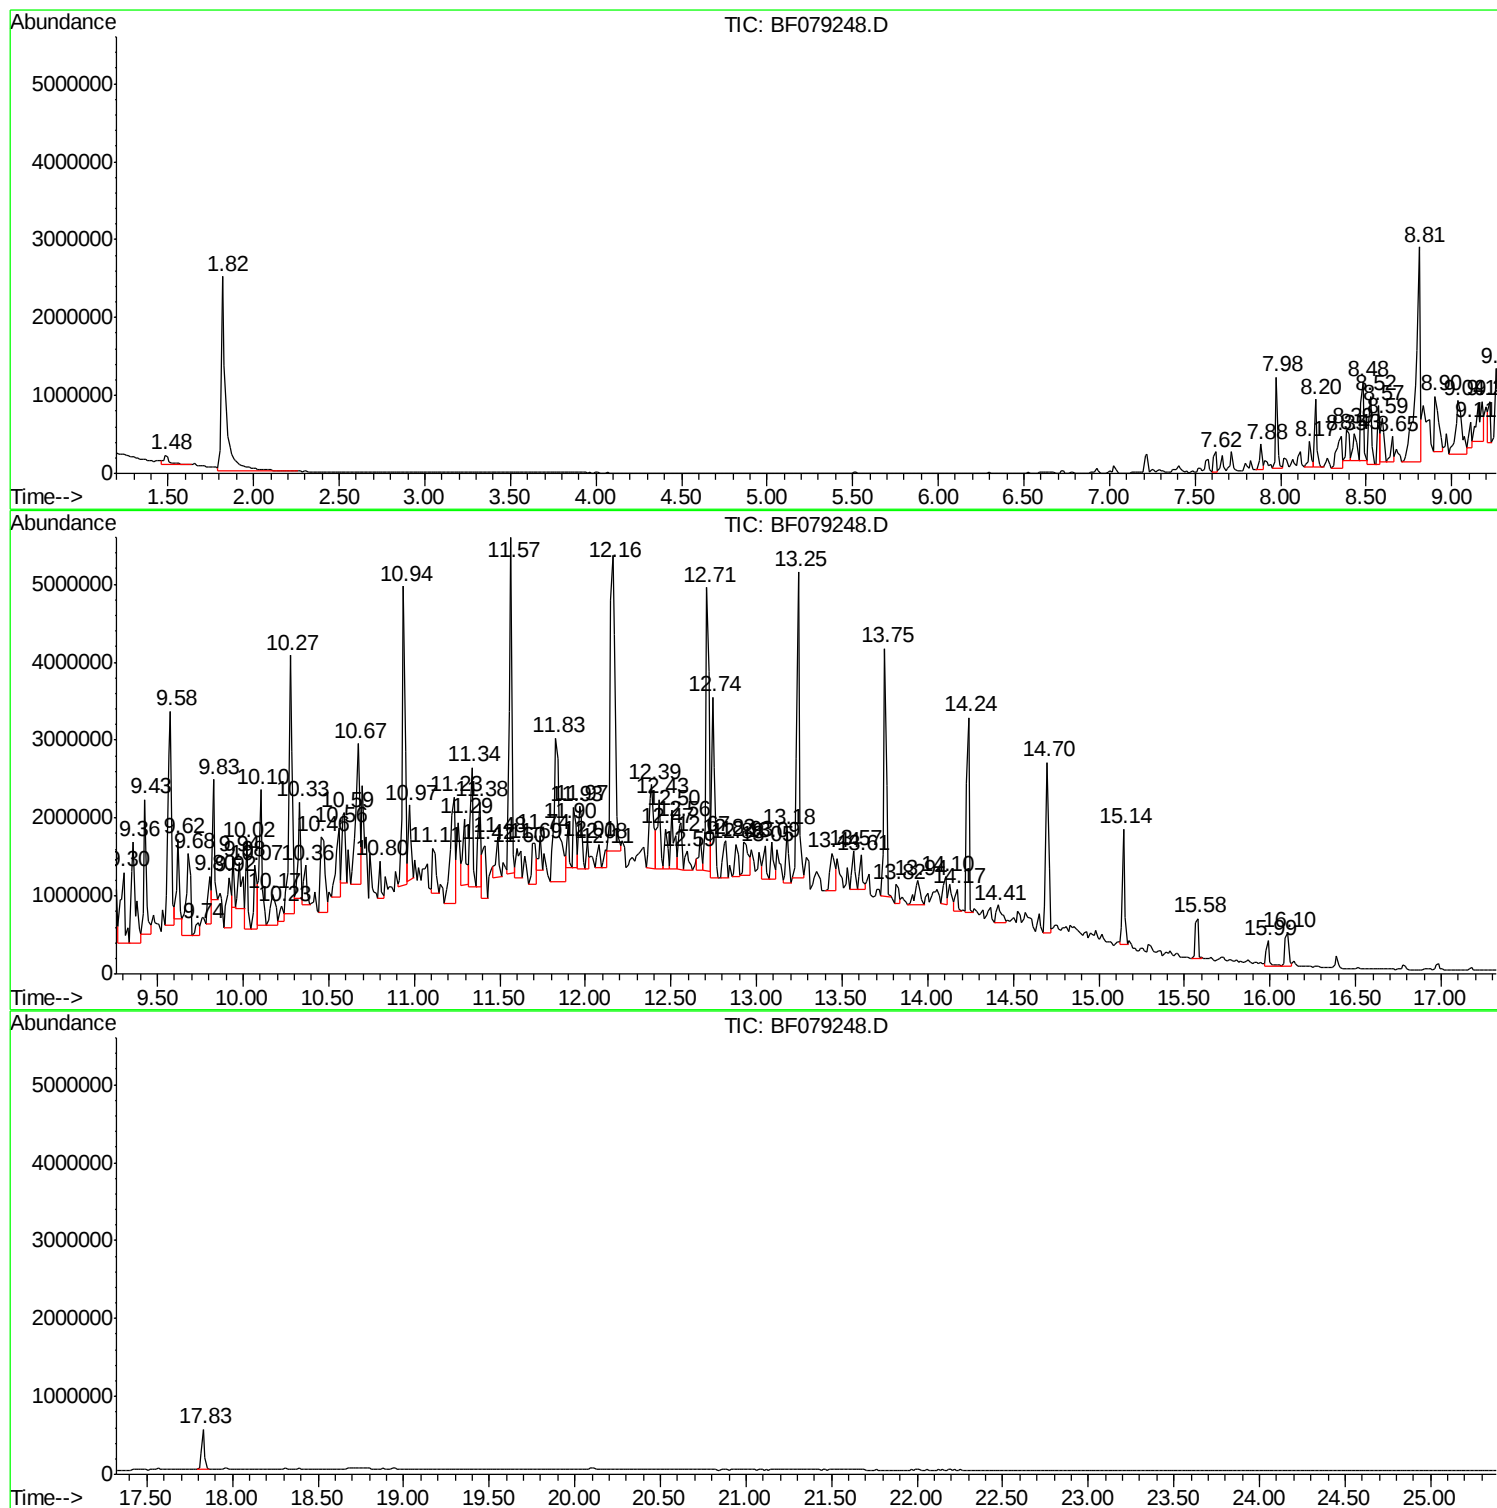

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF051415\
Data_File : BF079248.D
Acq_On : 14 May, 2015 23:122
Operator : TP/IZZ
Sample : G2201-03DL_25XX
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SUMP1DL

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
