


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051415\  
 Data File : BF079235.D  
 Acq On : 14 May 2015 14:13  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF043015.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri May 15 01:57:52 2015

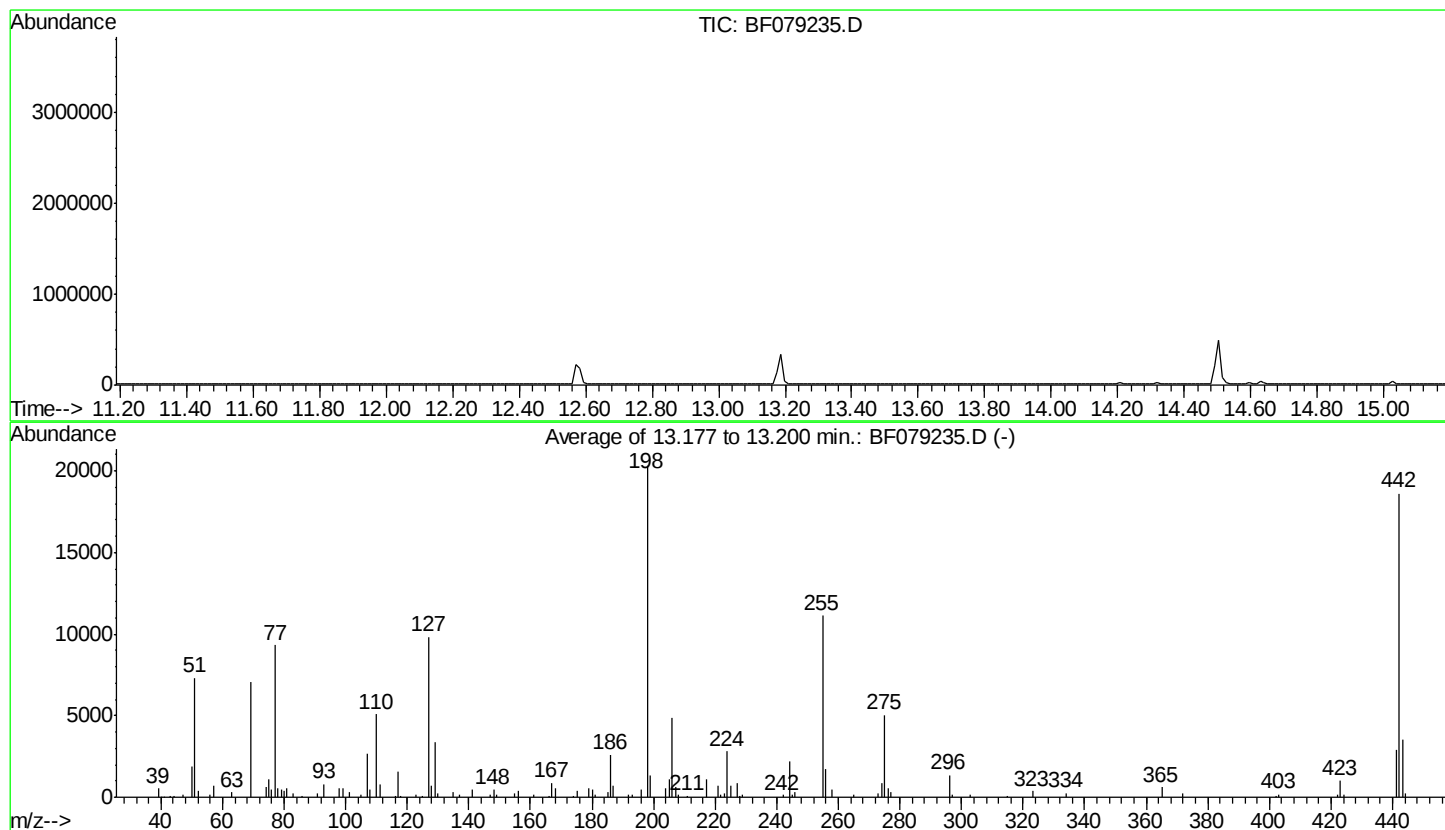

AutoFind: Scans 1049, 1050, 1051; Background Corrected with Scan 1046

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.9      | 7307    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 34.6      | 7042    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 48.4      | 9844    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 20329   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 1318    | PASS             |
| 275         | 198          | 10           | 60           | 24.9      | 5061    | PASS             |
| 365         | 198          | 1            | 100          | 3.0       | 614     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.5      | 2893    | PASS             |
| 442         | 198          | 50           | 100          | 91.7      | 18639   | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 3571    | PASS             |