


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051416\
 Data File : BF087026.D
 Acq On : 14 May 2016 18:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 13 14:55:23 2016

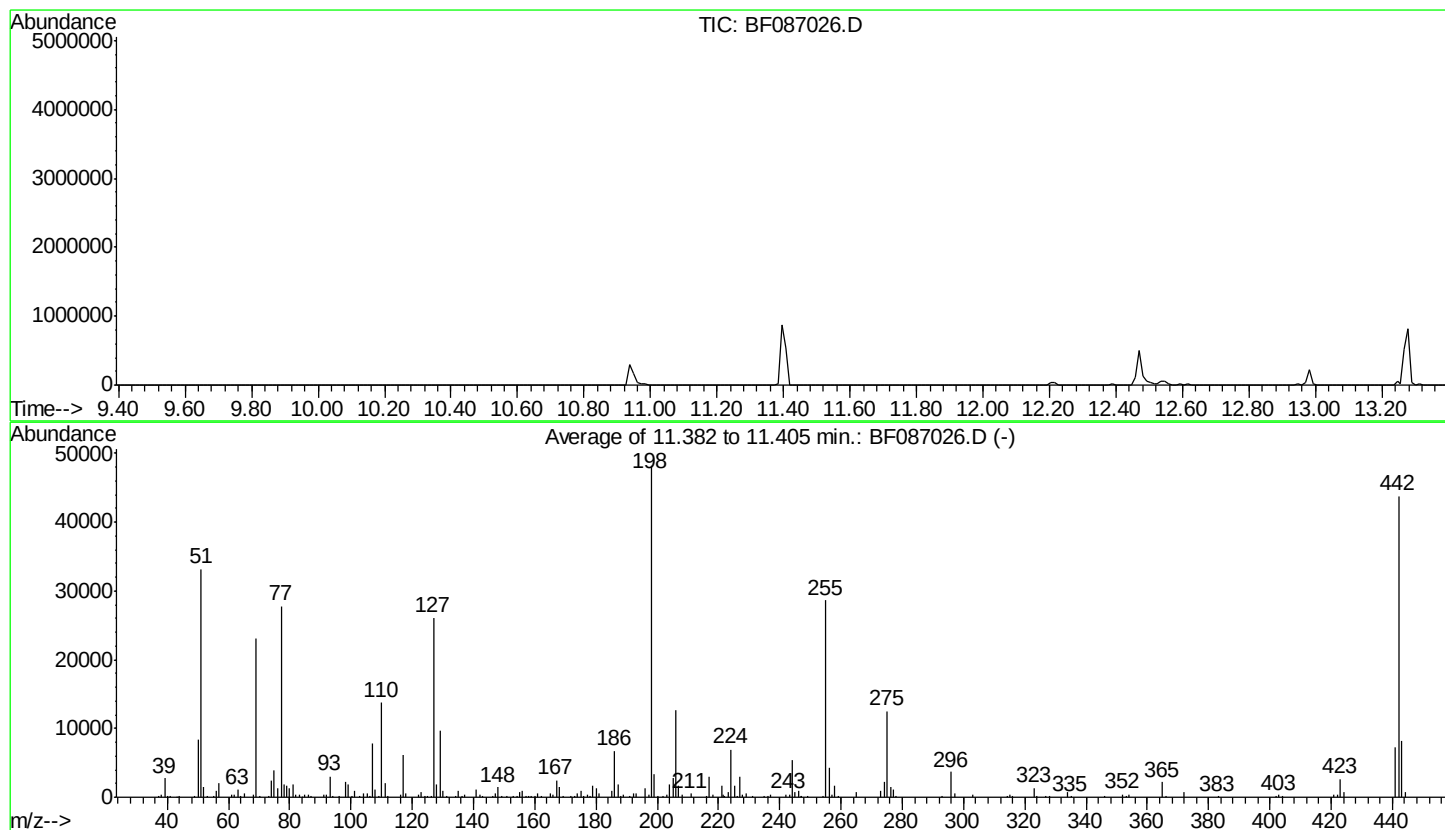

AutoFind: Scans 857, 858, 859; Background Corrected with Scan 854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.9	33211	PASS
68	69	0.00	2	1.7	393	PASS
69	198	0.00	100	48.0	23165	PASS
70	69	0.00	2	0.5	108	PASS
127	198	10	80	54.1	26079	PASS
197	198	0.00	2	0.7	357	PASS
198	198	100	100	100.0	48220	PASS
199	198	5	9	6.9	3338	PASS
275	198	10	60	26.0	12540	PASS
365	198	1	100	4.5	2157	PASS
441	442	0.01	24	16.4	7191	PASS
442	198	50	100	90.9	43837	PASS
443	442	15	24	18.7	8202	PASS