
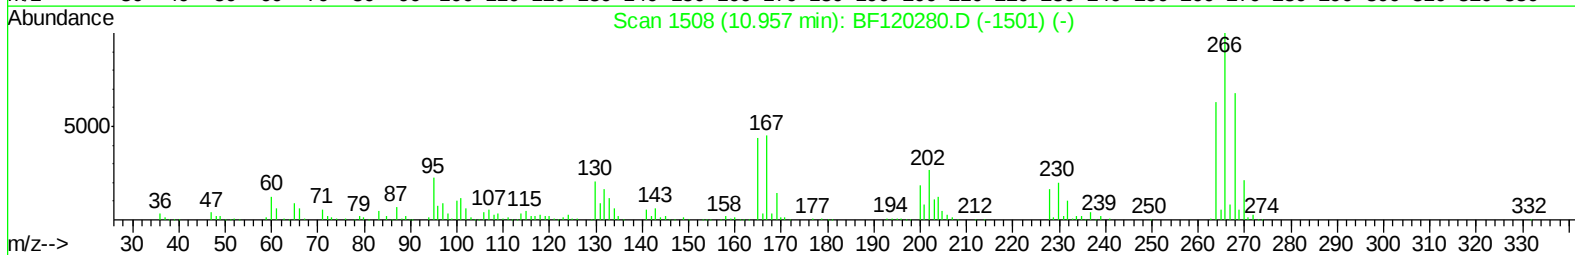
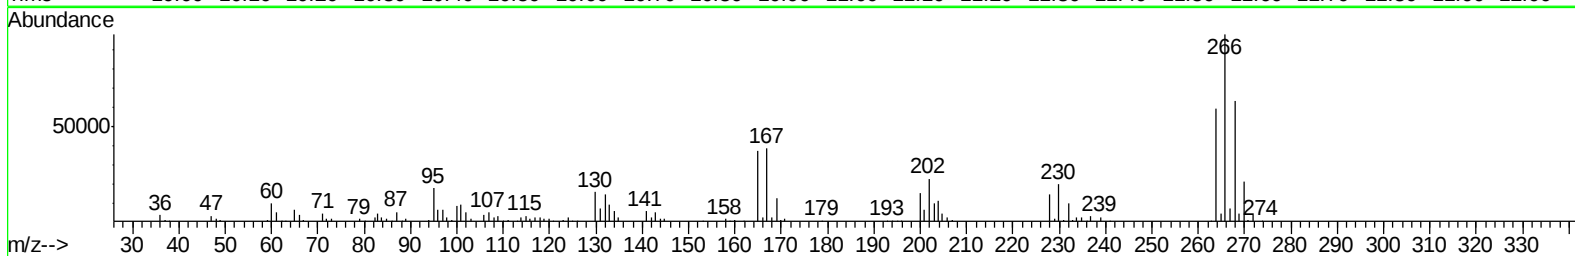


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF051420\
Data File : BF120277.D
Acq On : 14 May 2020 8:54
Operator : MA/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 07:35:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 12:47:38 2020
Response via : Initial Calibration

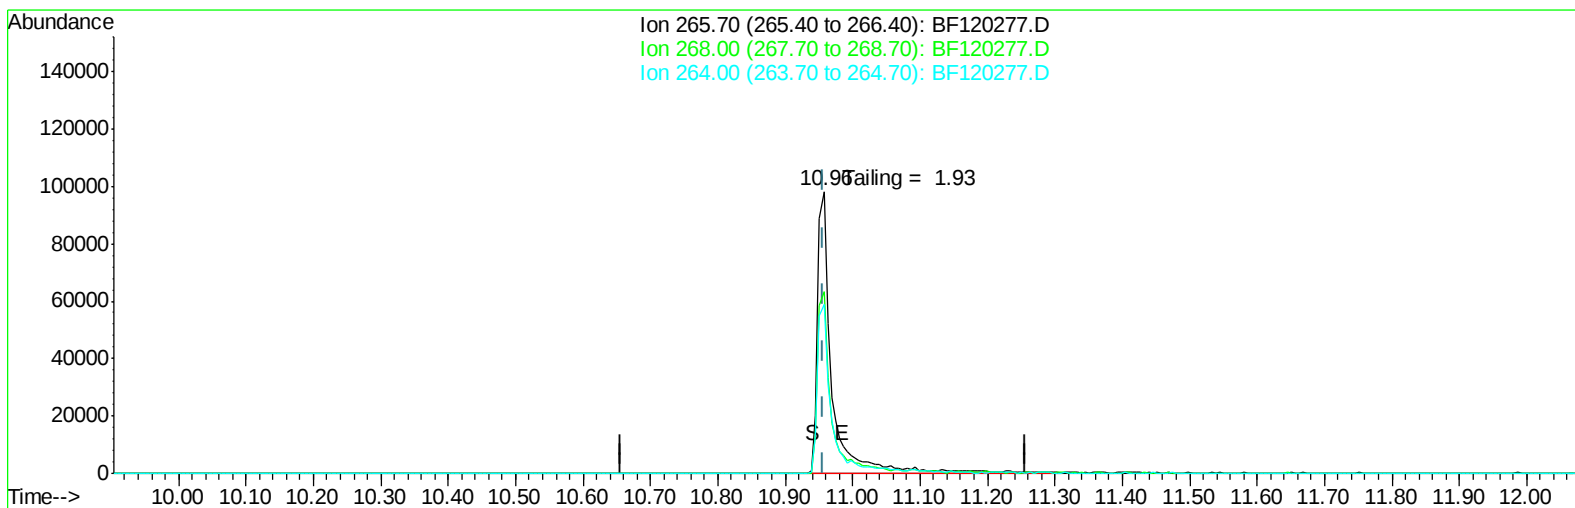

TIC: BF120277.D

(70) Pentachlorophenol (C)




10.957min (+0.000) 38600.28ng

response 133997

Ion	Exp%	Act%
265.70	100	100
268.00	67.80	64.37
264.00	62.80	60.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF051420\
 Data File : BF120277.D
 Acq On : 14 May 2020 8:54
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 07:35:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 14 12:47:38 2020
 Response via : Initial Calibration

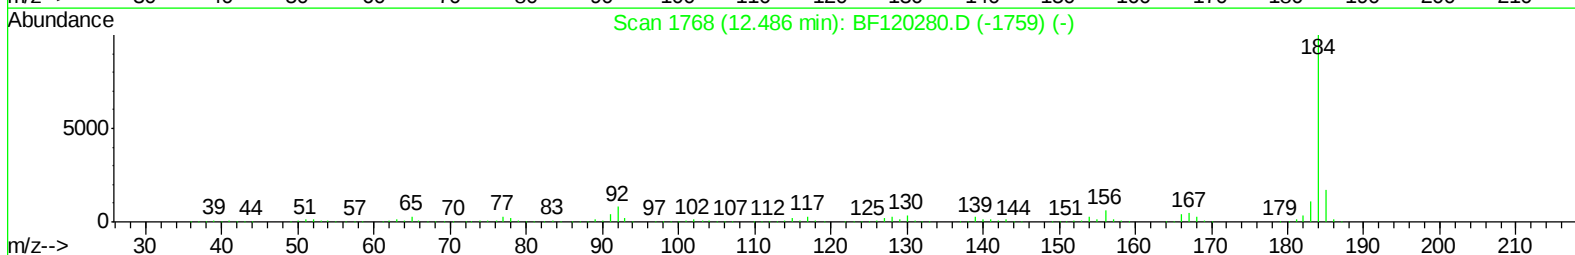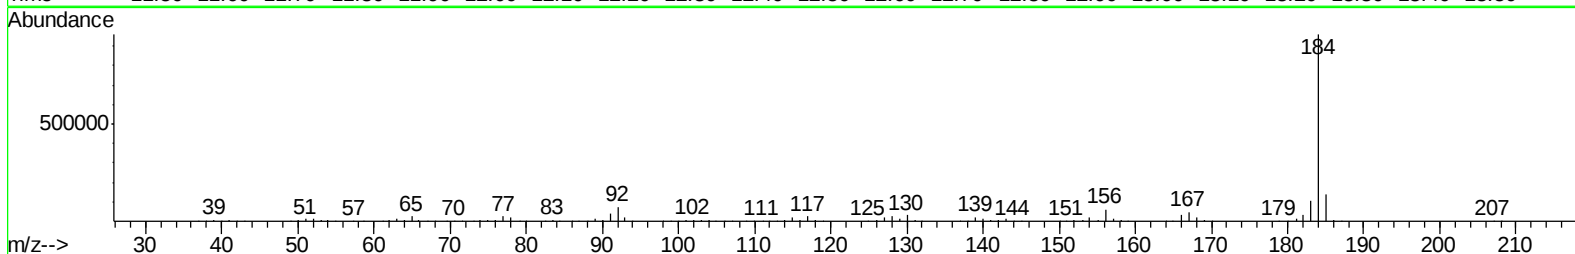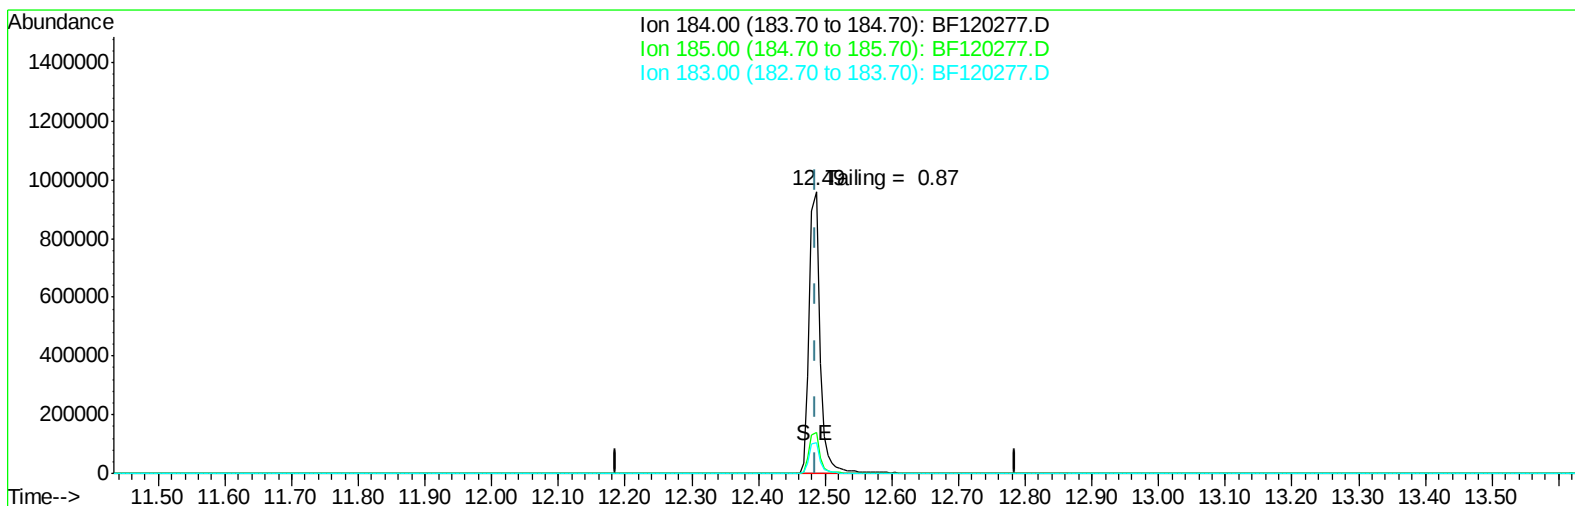

TIC: BF120277.D

(77) Benzidine

12.486min (+0.000) 0.00ng

response 1039902

Ion	Exp%	Act%
184.00	100	100
185.00	17.10	14.57
183.00	10.90	11.11
0.00	0.00	0.00