

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF051420\  
Data File : BF120288.D  
Acq On : 14 May 2020 14:10  
Operator : MA/SJ  
Sample : PB128845BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB128845BL

Integration Parameters: rteint.p  
Integrator: RTE  
Smoothing : ON Filtering: 5  
Sampling : 1 Min Area: 3 % of largest Peak  
Start Thrs: 0.2 Max Peaks: 100  
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051420.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.228       | 530           | 534         | 561          | rBV      | 6981833        | 8084354       | 80.15%          | 11.016%       |
| 2         | 6.275       | 707           | 712         | 745          | rBV      | 6106658        | 8111924       | 80.43%          | 11.053%       |
| 3         | 6.622       | 767           | 771         | 793          | rBV      | 1653130        | 2056684       | 20.39%          | 2.802%        |
| 4         | 6.775       | 793           | 797         | 826          | rVB      | 5626004        | 6812508       | 67.54%          | 9.283%        |
| 5         | 7.192       | 863           | 868         | 889          | rBV      | 4615203        | 5583163       | 55.35%          | 7.608%        |
| 6         | 7.904       | 985           | 989         | 1013         | rBV      | 2385721        | 2852186       | 28.28%          | 3.886%        |
| 7         | 8.986       | 1167          | 1173        | 1188         | rBV      | 8547148        | 10025777      | 99.40%          | 13.661%       |
| 8         | 9.657       | 1282          | 1287        | 1312         | rBV      | 3257033        | 3337138       | 33.09%          | 4.547%        |
| 9         | 10.451      | 1417          | 1422        | 1450         | rBV      | 5353605        | 6292871       | 62.39%          | 8.575%        |
| 10        | 11.145      | 1536          | 1540        | 1566         | rVB      | 3241152        | 3597365       | 35.67%          | 4.902%        |
| 11        | 12.739      | 1805          | 1811        | 1814         | rBV      | 8763566        | 10086319      | 100.00%         | 13.743%       |
| 12        | 13.780      | 1984          | 1988        | 2001         | rBV      | 3478281        | 3483645       | 34.54%          | 4.747%        |
| 13        | 15.174      | 2219          | 2225        | 2235         | rBV      | 2372156        | 3066271       | 30.40%          | 4.178%        |


Sum of corrected areas: 73390205

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF051420\  
Data File : BF120288.D  
Acq On : 14 May 2020 14:10  
Operator : MA/SJ  
Sample : PB128845BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB128845BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

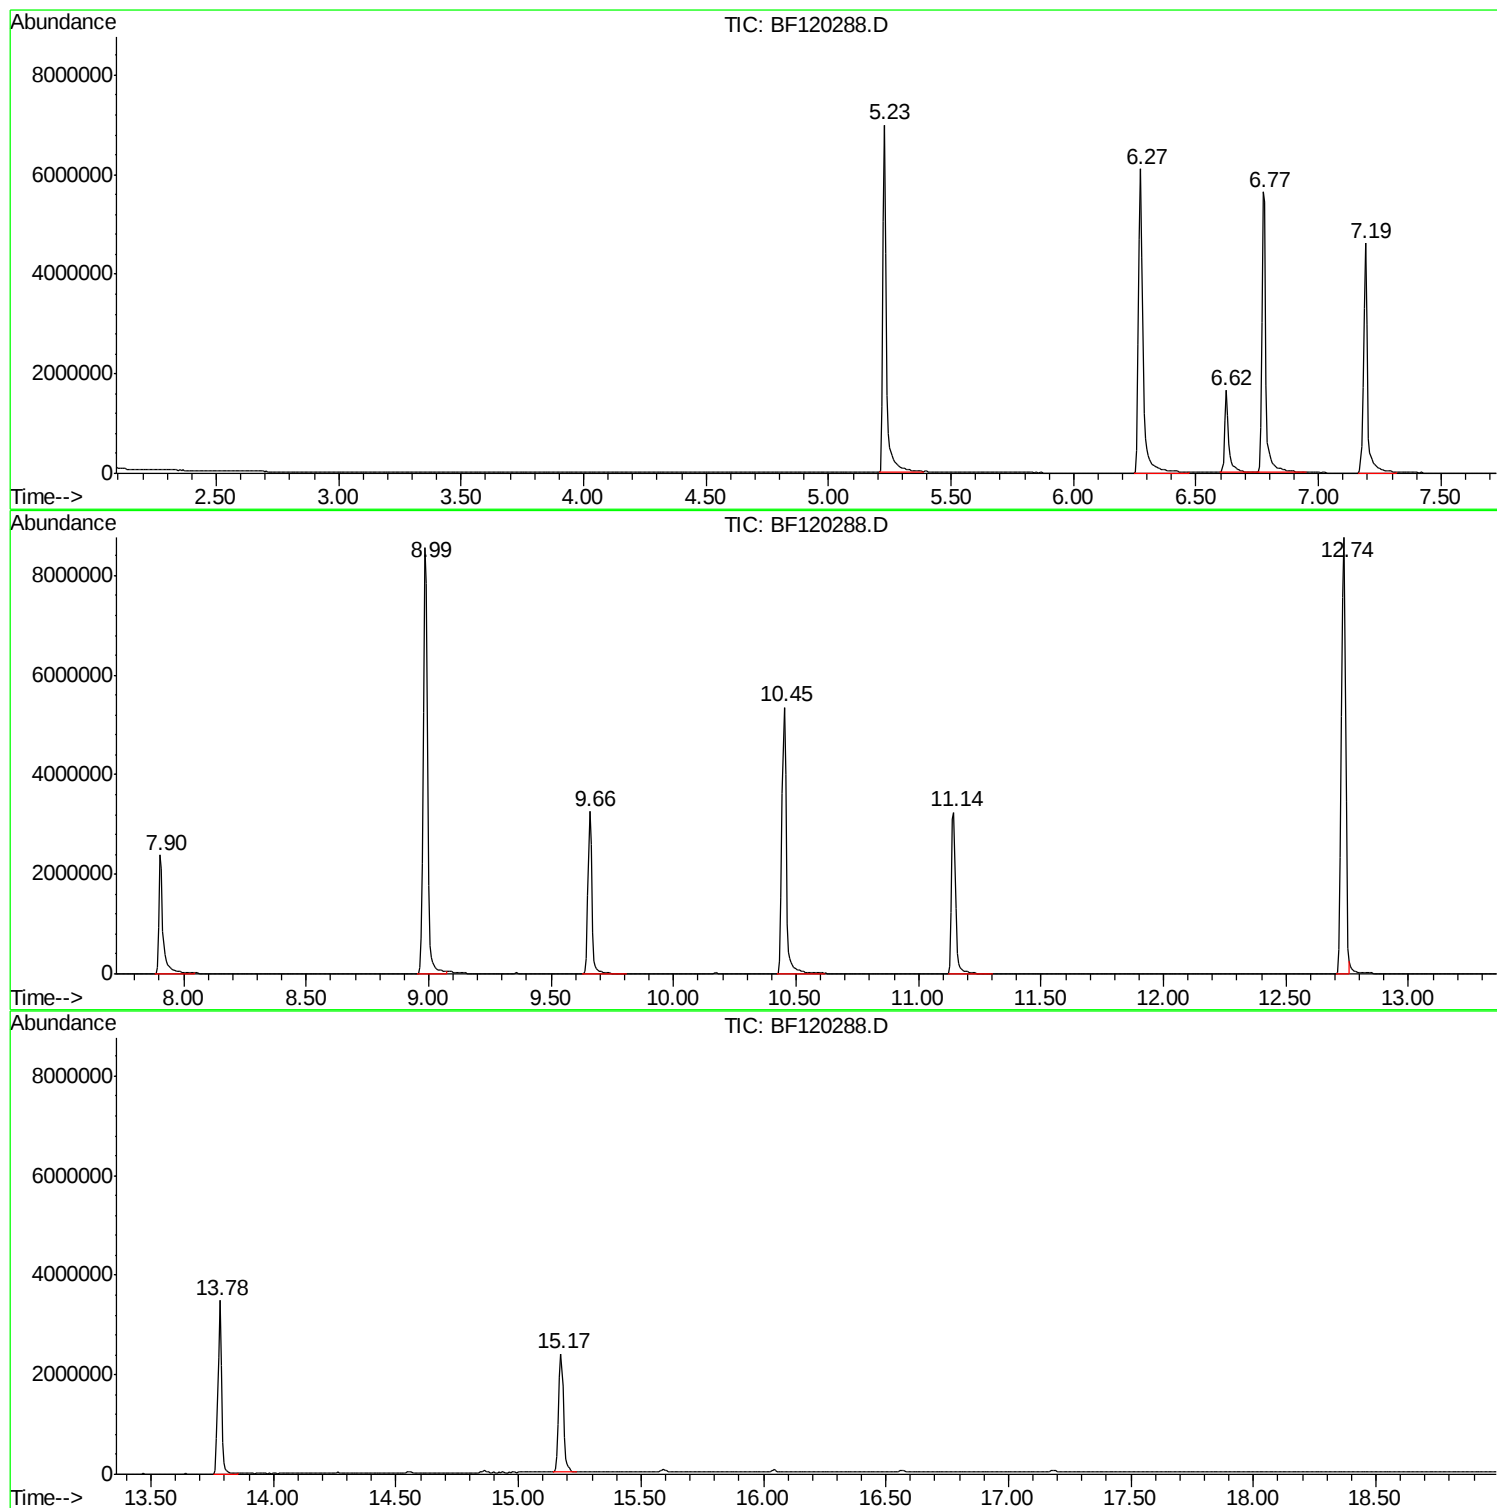

Data\_Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF051420\  
Data\_File : BF120288.D  
Acq\_On : 14 May, 2020 14:100  
Operator : MA/SJJ  
Sample : PB128845BLL  
Misc :  
ALS\_Vial : 3 Sample\_Multiplier: 11

Instrument :  
BNA\_F  
ClientSampleId :  
PB128845BL

Quant\_Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051420.MM  
Quant\_Title : ASP\_BNA\_STANDARDS\_FOR\_5\_POINT\_CALIBRATIONN

TIC\_Library : C:\DATABASE\NIST11.LL  
TIC\_Integration\_Parameters: LSCINT.PP

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|

No Library Search Compounds Detected

\*\*\*\*\*