

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051420\
 Data File : BF120290.D
 Acq On : 14 May 2020 15:04
 Operator : MA/SJ
 Sample : PB128891BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128891BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.228	530	534	565	rBV	5240353	6201141	76.83%	10.404%
2	6.275	707	712	749	rBV	4852131	6156183	76.27%	10.329%
3	6.622	767	771	793	rBV	1601305	1954109	24.21%	3.279%
4	6.775	793	797	824	rVV	4693523	5142037	63.70%	8.627%
5	7.192	863	868	899	rBV	3719168	4388999	54.38%	7.364%
6	7.904	985	989	1008	rBV	2159378	2613829	32.38%	4.385%
7	8.986	1168	1173	1188	rBV	7686958	7957602	98.59%	13.351%
8	9.657	1283	1287	1304	rBV	3395620	3207585	39.74%	5.382%
9	10.451	1417	1422	1449	rBV	4264003	4691033	58.12%	7.870%
10	11.139	1535	1539	1548	rBV	3292081	3628953	44.96%	6.089%
11	12.733	1805	1810	1827	rBV	7283186	8071639	100.00%	13.542%
12	13.780	1983	1988	1998	rBV	2897188	2952610	36.58%	4.954%
13	15.174	2219	2225	2239	rBV	2047151	2637149	32.67%	4.425%


Sum of corrected areas: 59602869

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF051420\
Data File : BF120290.D
Acq On : 14 May 2020 15:04
Operator : MA/SJ
Sample : PB128891BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128891BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

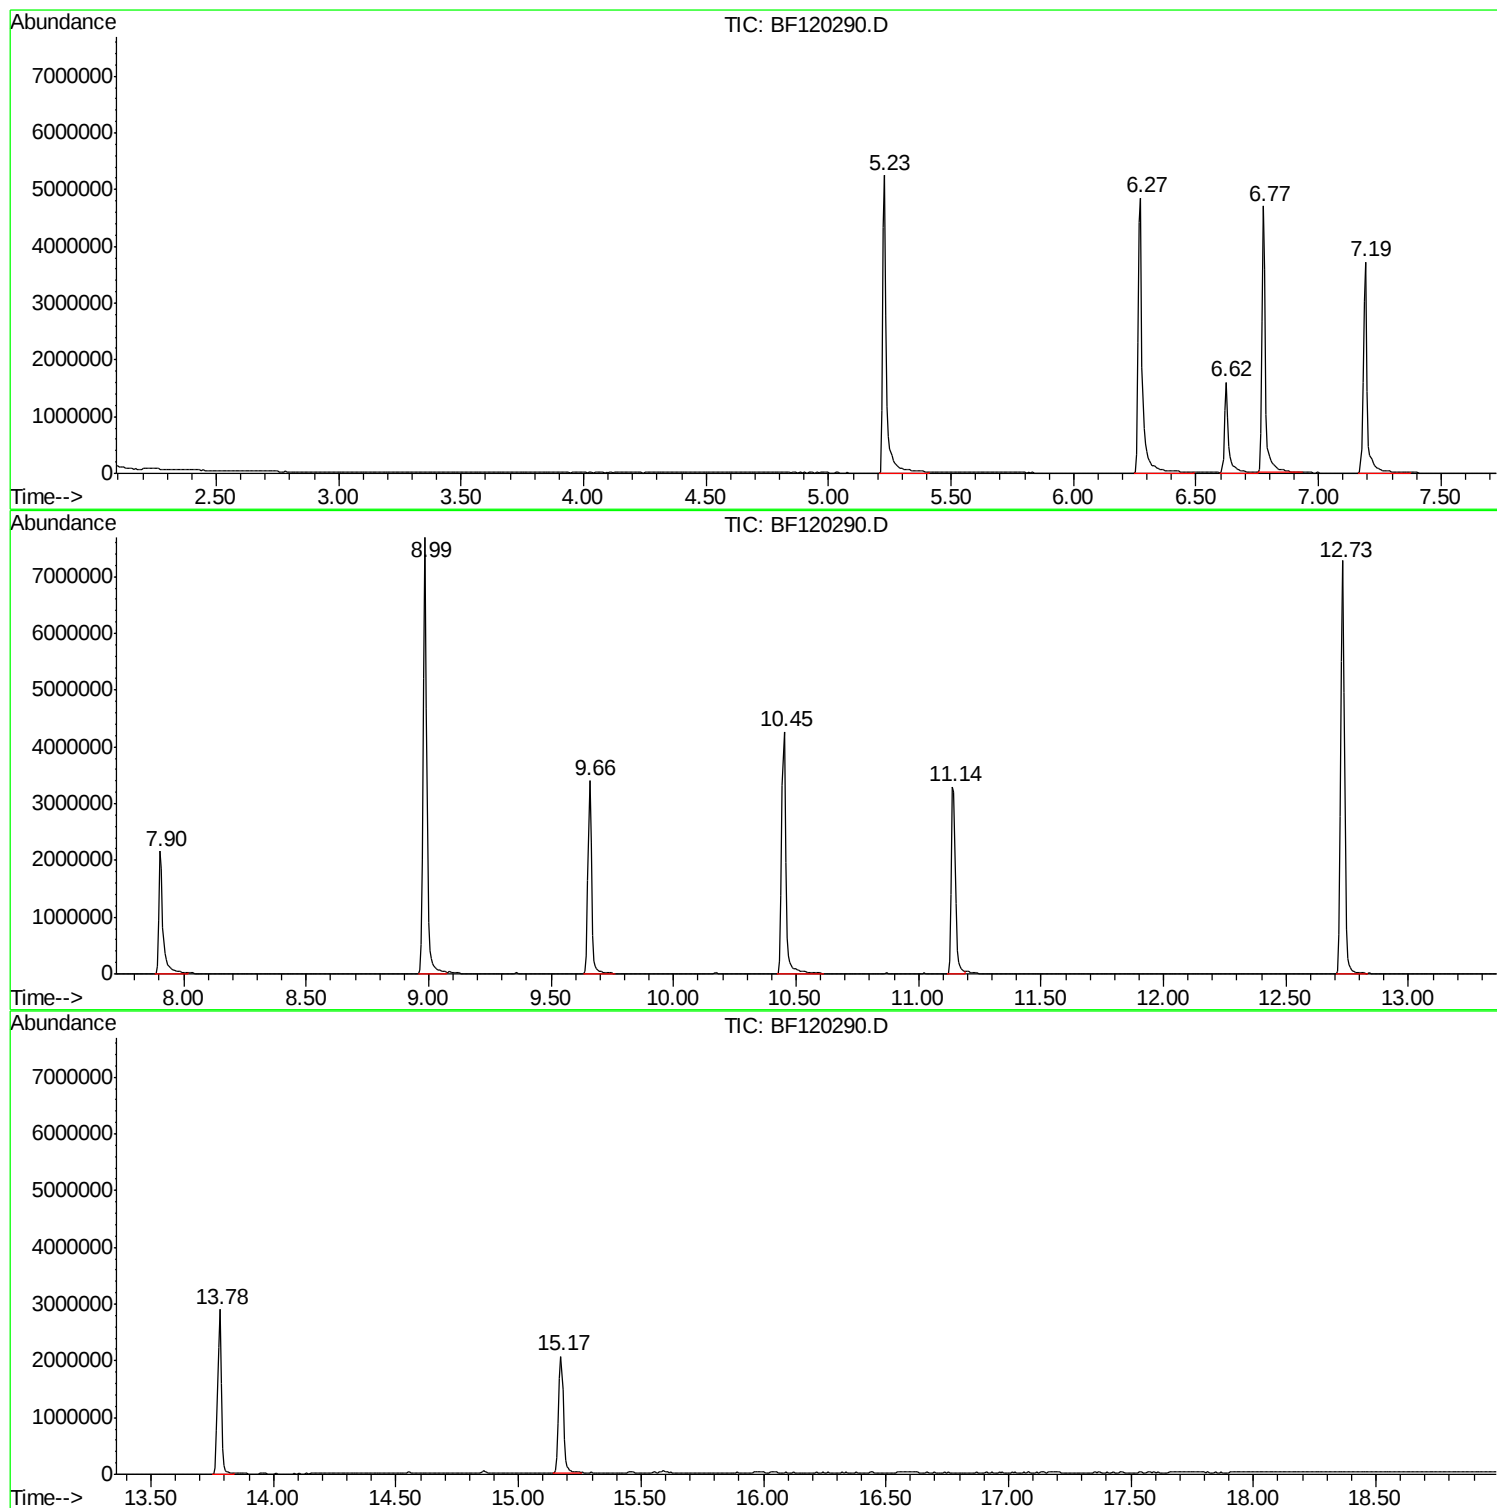

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051420\
Data_File : BF120290.D
Acq_On : 14 May, 2020 15:044
Operator : MA/SJJ
Sample : PB128891BLL
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB128891BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
