

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051420\
 Data File : BF120292.D
 Acq On : 14 May 2020 15:58
 Operator : MA/SJ
 Sample : PB128874BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128874BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.228	530	534	560	rBV	5983115	6954318	67.73%	10.069%
2	6.275	707	712	732	rBV	5600783	6865578	66.87%	9.941%
3	6.622	767	771	793	rBV	1697398	2119051	20.64%	3.068%
4	6.775	793	797	822	rVV	5145396	5952185	57.97%	8.618%
5	7.192	863	868	893	rBV	4159265	4872059	47.45%	7.054%
6	7.904	986	989	1008	rBV	2496824	2904755	28.29%	4.206%
7	8.986	1168	1173	1188	rBV	8174400	8843429	86.13%	12.804%
8	9.657	1283	1287	1309	rBV	3634995	3530660	34.39%	5.112%
9	10.451	1417	1422	1448	rBV	5005680	5838594	56.87%	8.454%
10	11.139	1535	1539	1568	rBV	3568660	3967673	38.64%	5.745%
11	12.733	1805	1810	1832	rBV	8308829	10267151	100.00%	14.866%
12	13.780	1984	1988	2001	rBV	3619363	3625366	35.31%	5.249%
13	15.174	2219	2225	2237	rBV	2401862	3216422	31.33%	4.657%
14	15.462	2269	2274	2284	rVB7	39335	109029	1.06%	0.158%


Sum of corrected areas: 69066270

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051420\
Data File : BF120292.D
Acq On : 14 May 2020 15:58
Operator : MA/SJ
Sample : PB128874BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128874BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

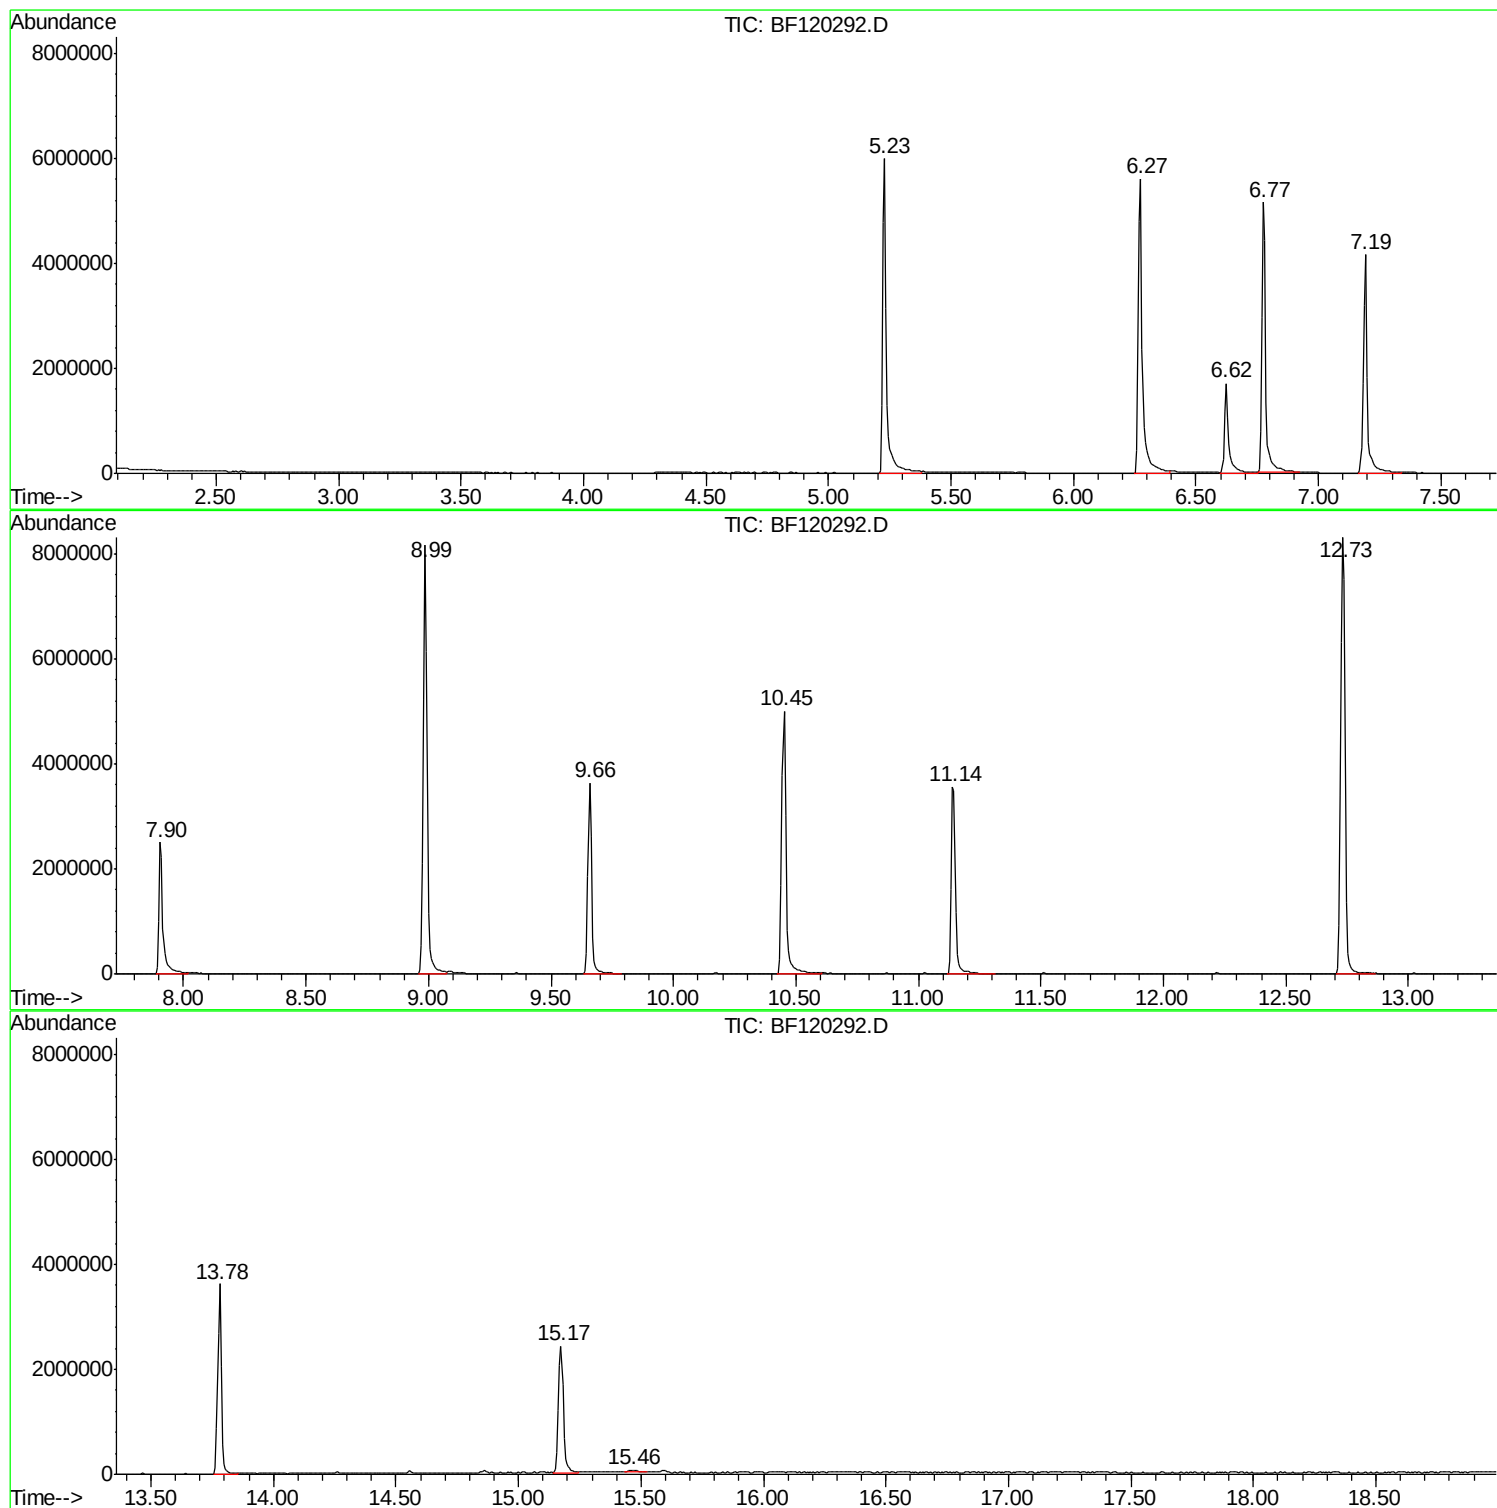

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051420\
Data File : BF120292.D
Acq On : 14 May 2020 15:58
Operator : MA/SJ
Sample : PB128874BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128874BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051420\
Data File : BF120292.D
Acq On : 14 May 2020 15:58
Operator : MA/SJ
Sample : PB128874BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128874BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc