


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051420\
 Data File : BF120277.D
 Acq On : 14 May 2020 8:54
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 14 12:47:38 2020

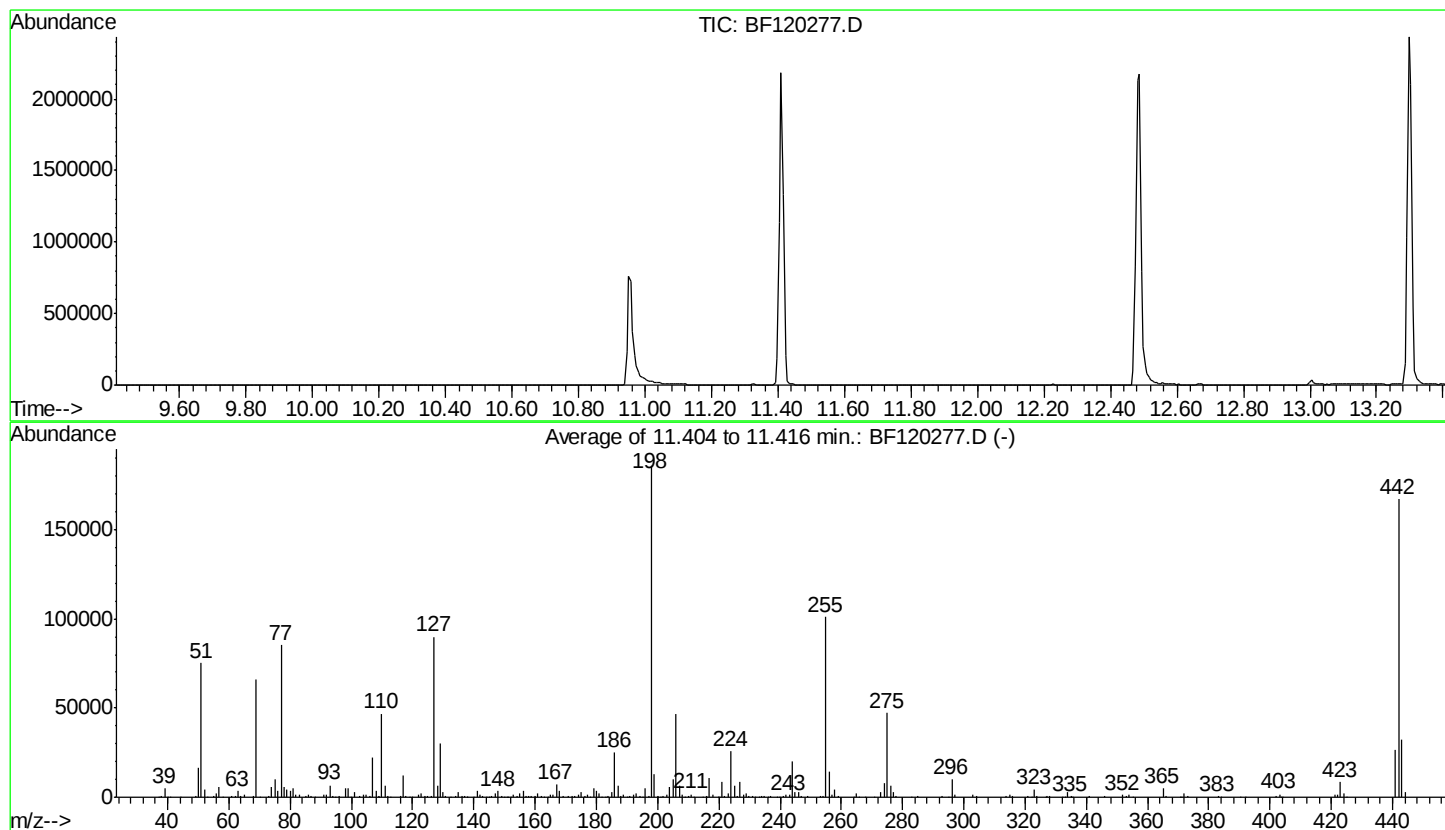

AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	75277	PASS
68	69	0.00	2	1.6	1070	PASS
69	198	0.00	100	35.5	65920	PASS
70	69	0.00	2	0.5	310	PASS
127	198	10	80	48.4	90048	PASS
197	198	0.00	2	0.3	593	PASS
198	198	100	100	100.0	185877	PASS
199	198	5	9	7.0	12997	PASS
275	198	10	60	25.3	47072	PASS
365	198	1	100	2.5	4725	PASS
441	198	0.01	100	14.3	26666	PASS
442	198	50	100	89.8	166941	PASS
443	442	15	24	19.4	32451	PASS