


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051420\
 Data File : BF120286.D
 Acq On : 14 May 2020 13:17
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 14 12:47:38 2020

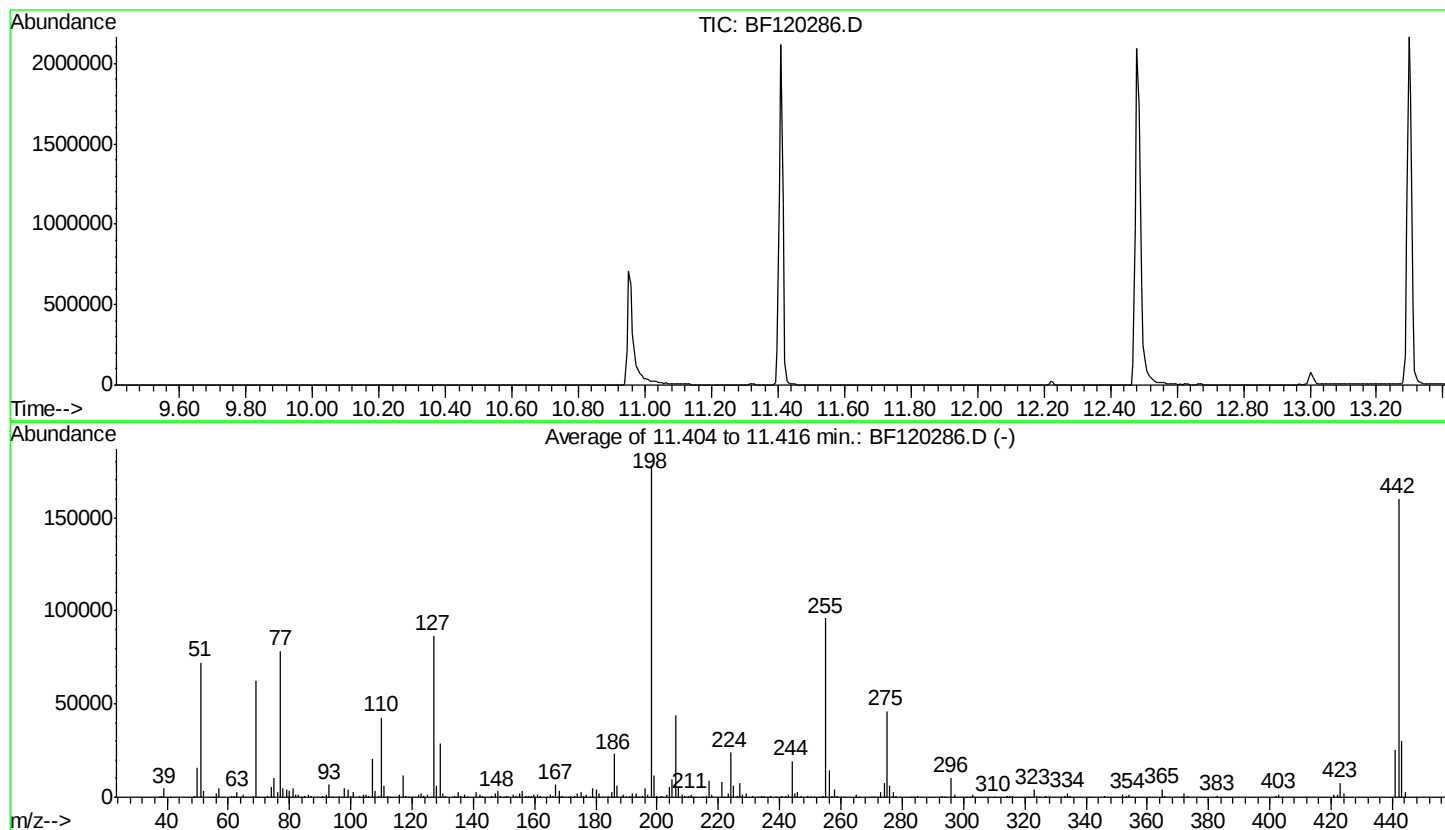

AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	72357	PASS
68	69	0.00	2	1.3	827	PASS
69	198	0.00	100	35.2	62592	PASS
70	69	0.00	2	0.5	335	PASS
127	198	10	80	48.8	86728	PASS
197	198	0.00	2	0.7	1175	PASS
198	198	100	100	100.0	177858	PASS
199	198	5	9	6.7	11903	PASS
275	198	10	60	26.0	46288	PASS
365	198	1	100	2.4	4284	PASS
441	198	0.01	100	14.3	25461	PASS
442	198	50	100	90.1	160253	PASS
443	442	15	24	18.7	30001	PASS