
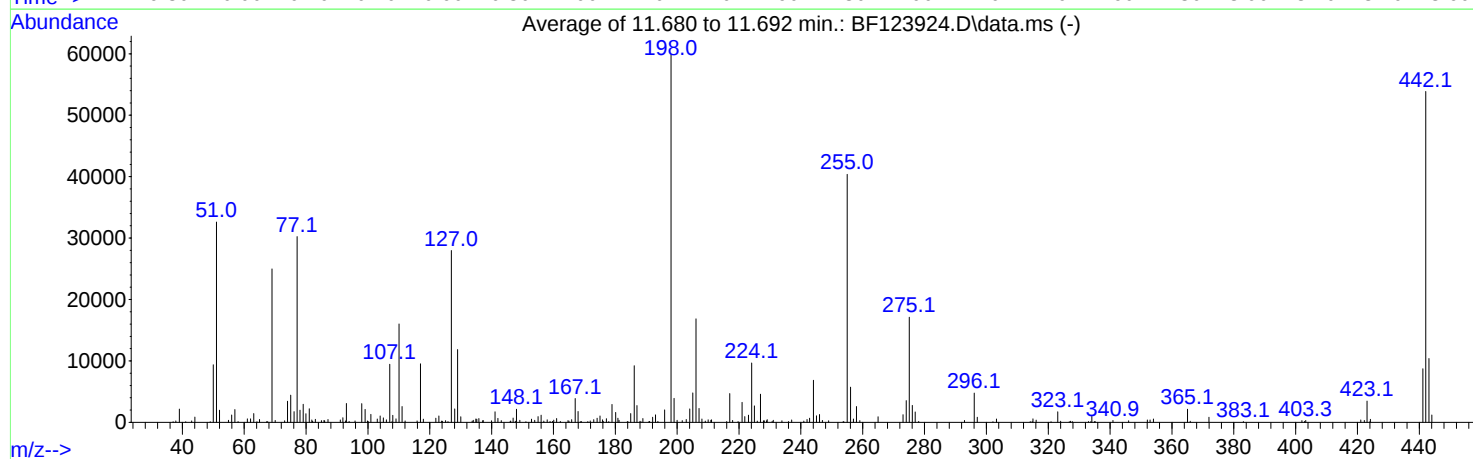


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051421\
 Data File : BF123924.D
 Acq On : 14 May 2021 13:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 14 19:05:57 2021

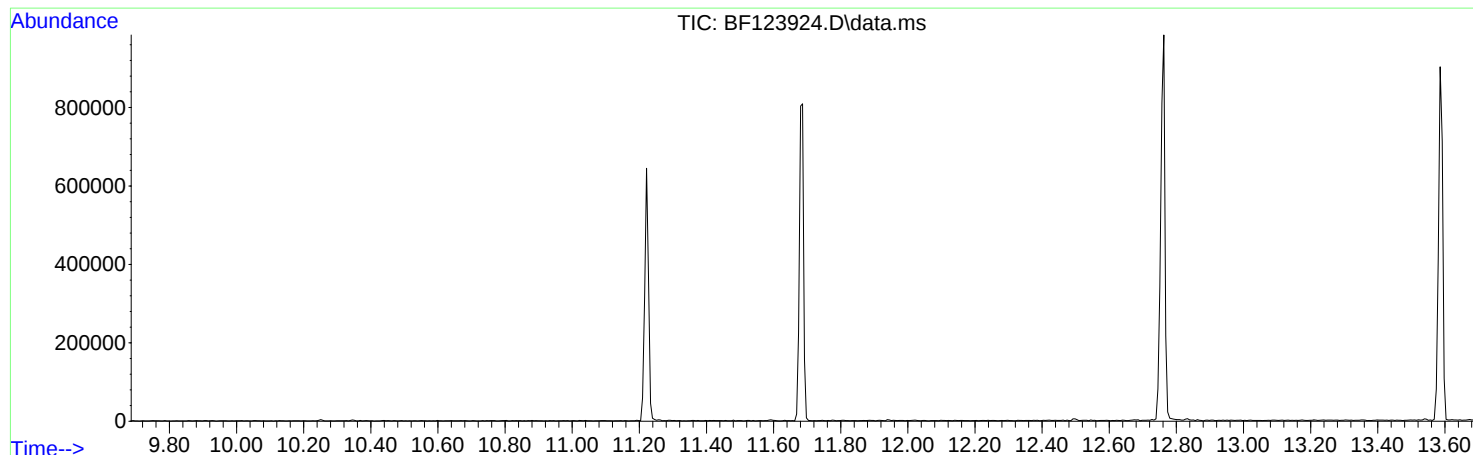




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	32614	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.7	24993	PASS
70	69	0.00	2	1.2	305	PASS
127	198	10	80	46.7	27965	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59885	PASS
199	198	5	9	6.5	3898	PASS
275	198	10	60	28.6	17125	PASS
365	198	1	100	3.6	2145	PASS
441	198	0.01	100	14.6	8734	PASS
442	442	50	100	100.0	53869	PASS
443	442	15	24	19.3	10399	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051421\
Data File : BF123924.D
Acq On : 14 May 2021 13:22
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 14 15:24:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:09:51 2021
Response via : Initial Calibration

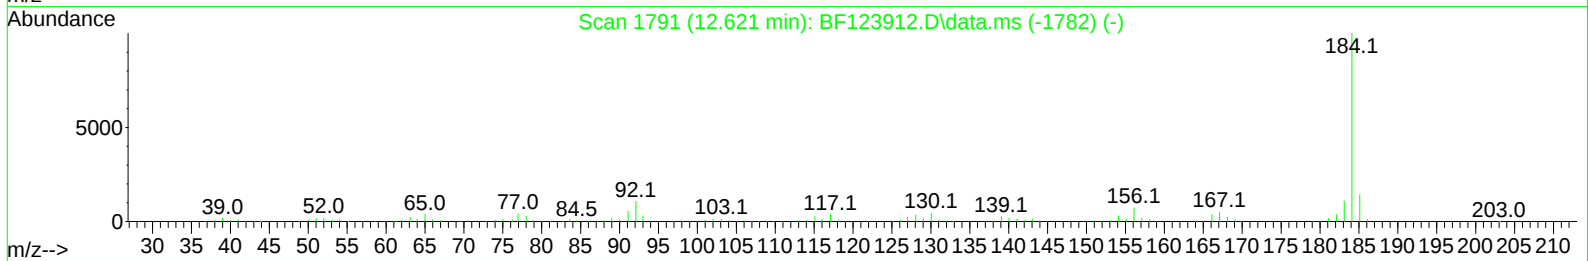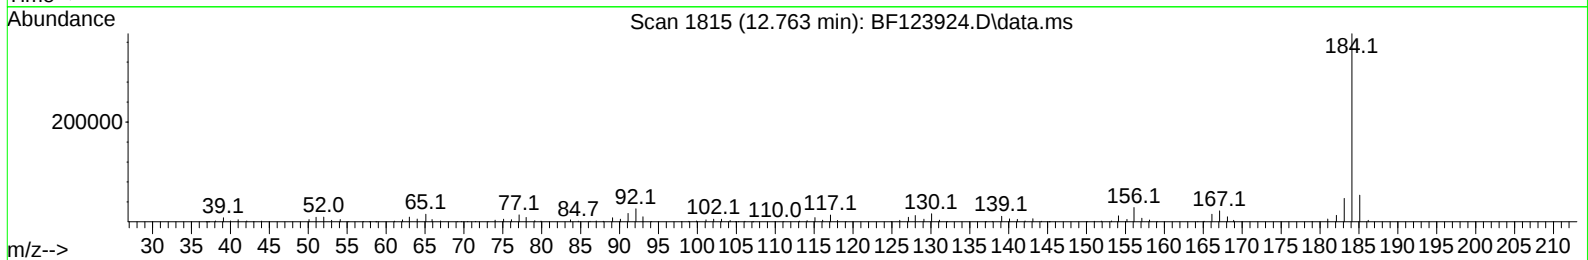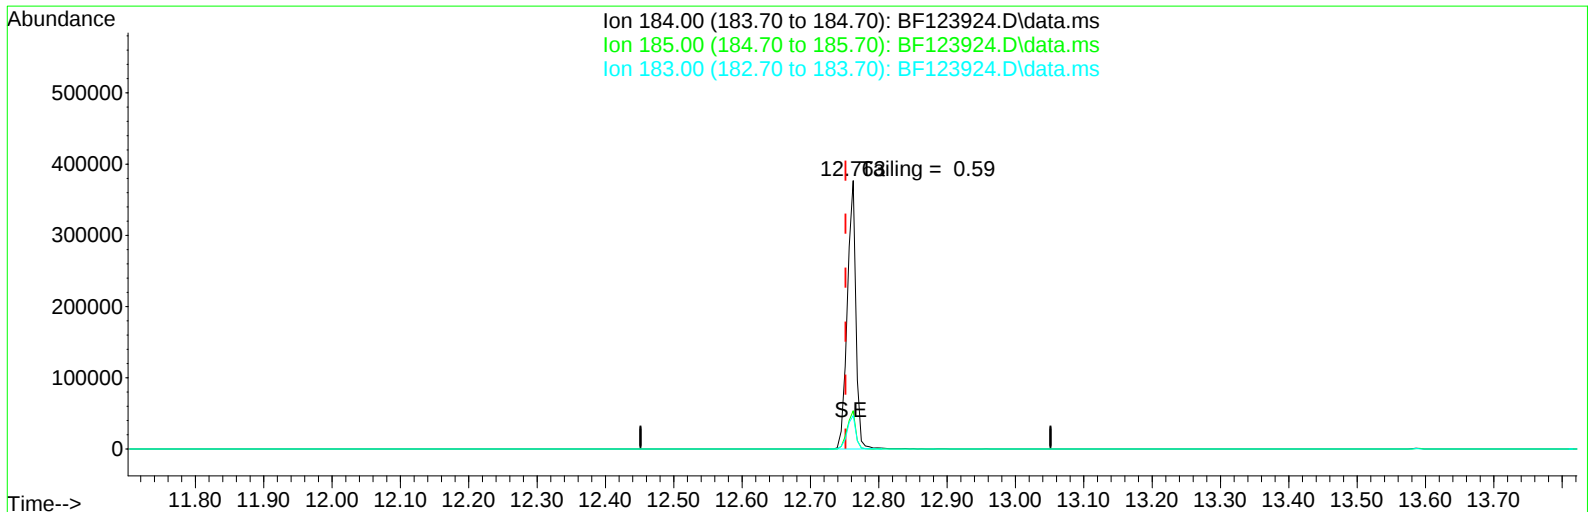

TIC: BF123924.D\data.ms

(77) Benzidine

12.763min (+ 0.011) 0.00 ng




response 326617

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.24
183.00	9.80	12.47#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051421\
Data File : BF123924.D
Acq On : 14 May 2021 13:22
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 14 15:24:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 15:09:51 2021
Response via : Initial Calibration

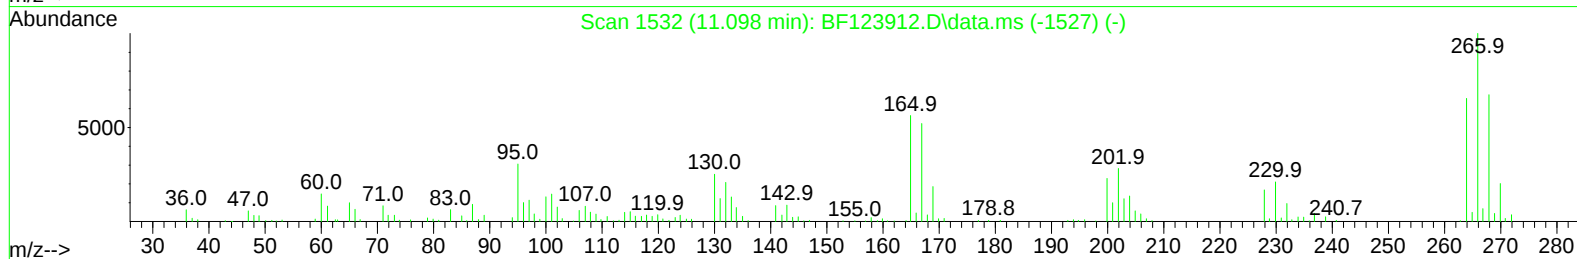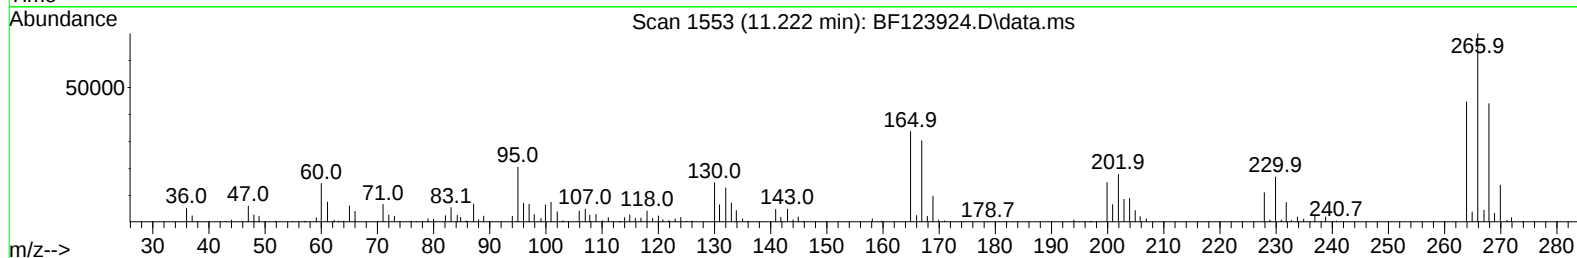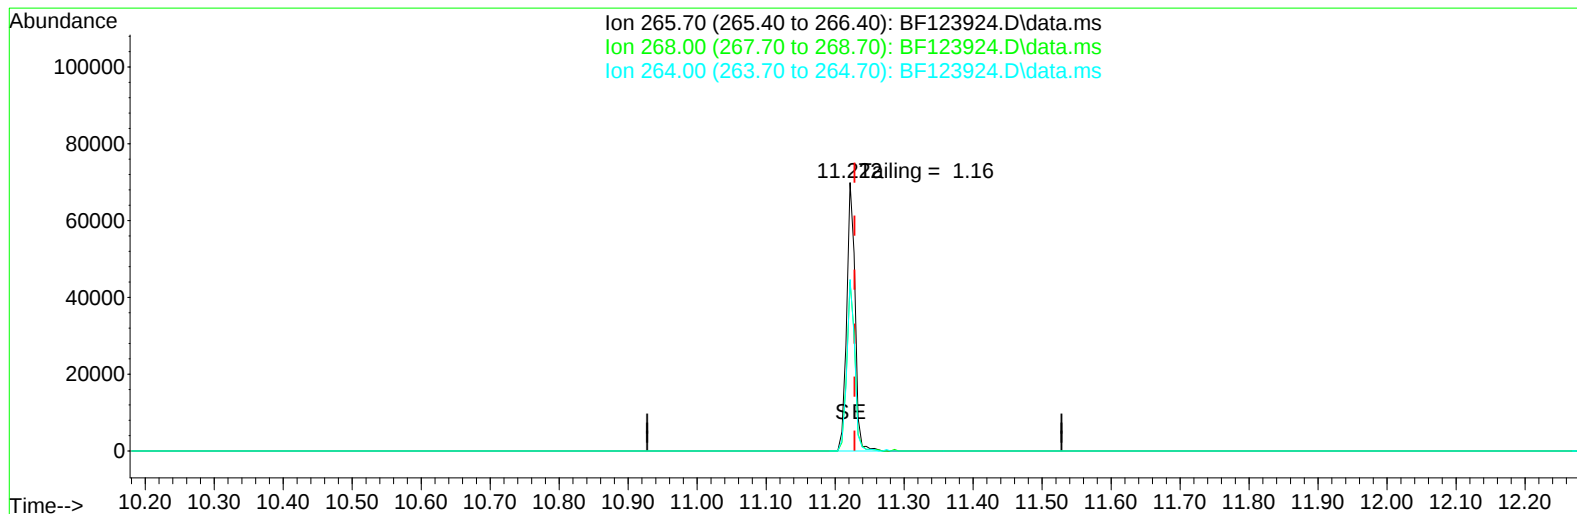

TIC: BF123924.D\data.ms

(70) Pentachlorophenol (C)

11.222min (-0.006) 46579.39 ng

response 58797

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.99
264.00	65.70	63.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/14/2021	BNA_F	BF123924.D
Compound Name	Response	Retention Time
DDT	130178	13.58
DDD	121	13.14
DDE	126	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
247	130425	0.19