
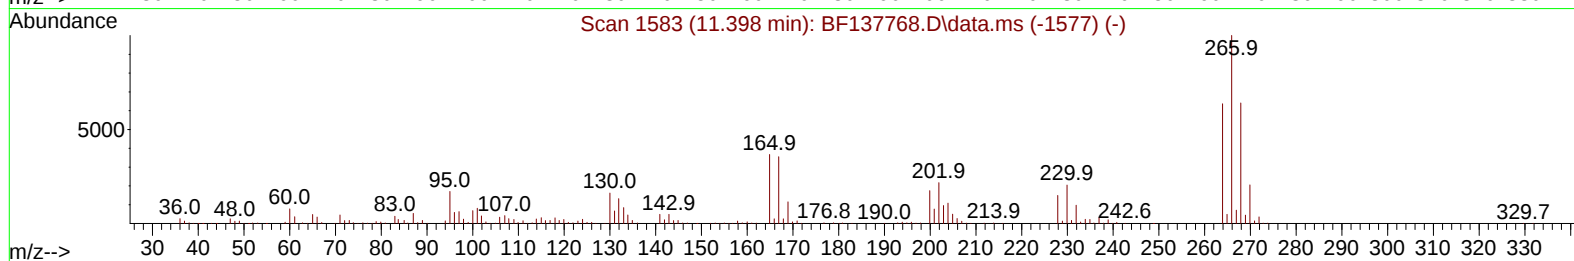
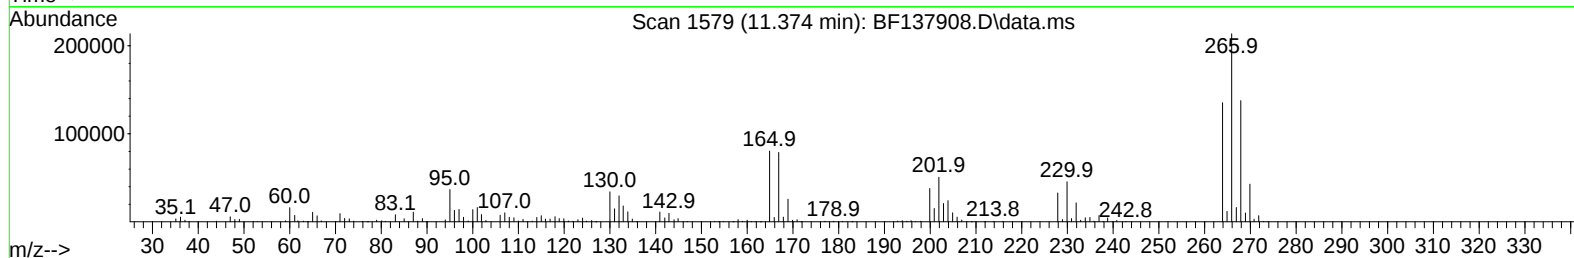


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051424\
Data File : BF137908.D
Acq On : 14 May 2024 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 12:38:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

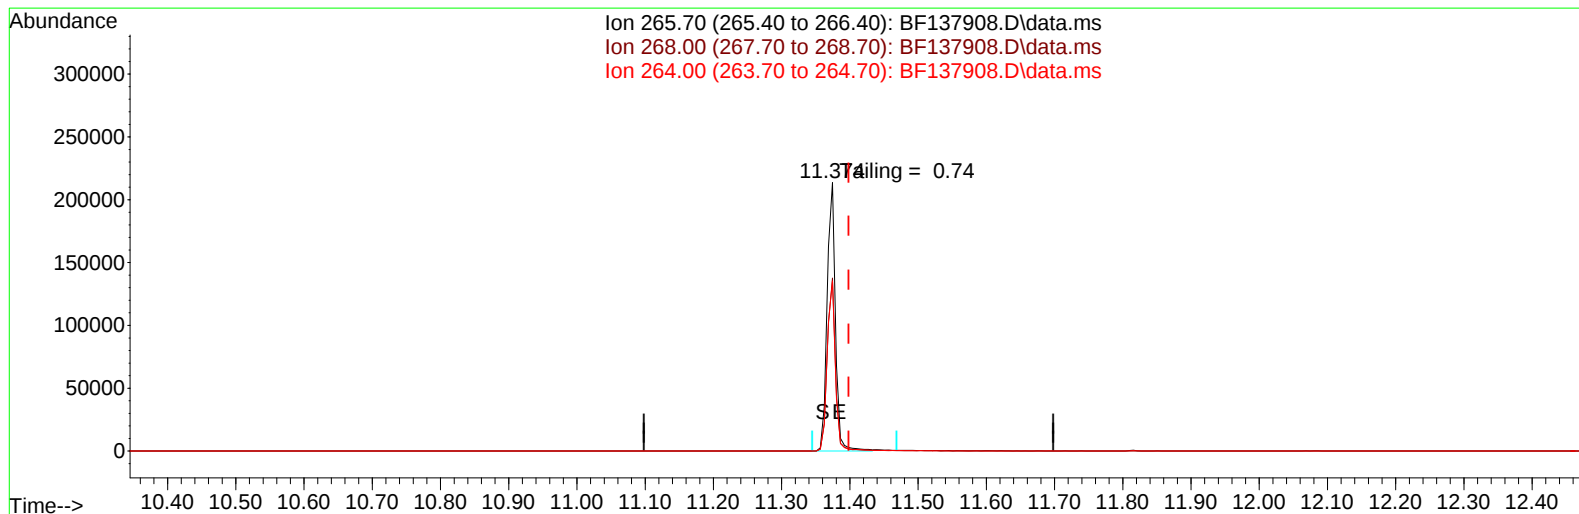

TIC: BF137908.D\data.ms

(70) Pentachlorophenol (C)




11.374min (-0.024) 27547.94 ng

response 181379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.44
264.00	63.70	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051424\
Data File : BF137908.D
Acq On : 14 May 2024 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 12:38:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

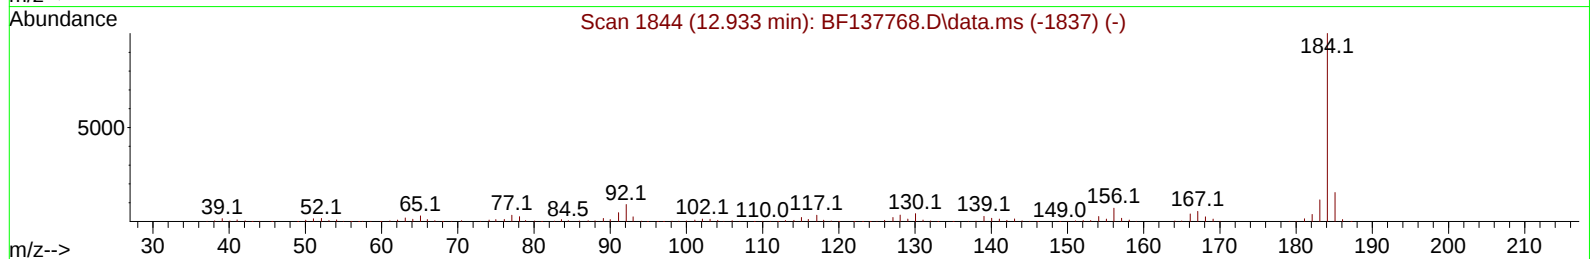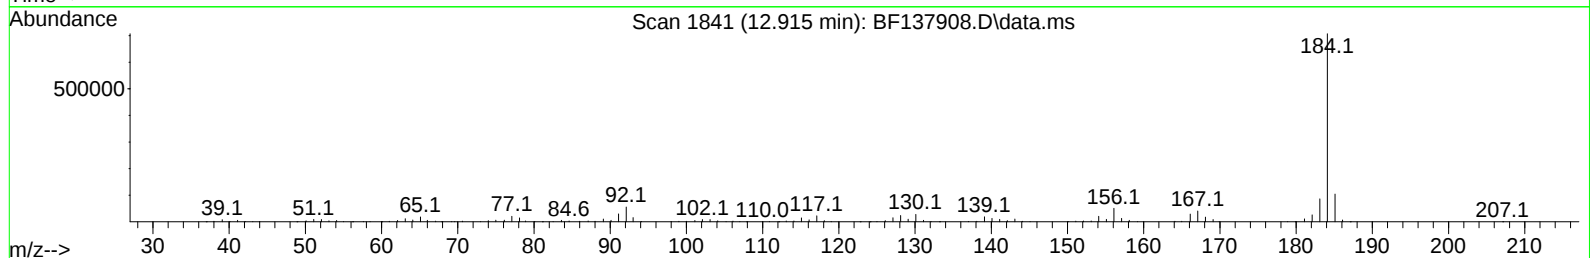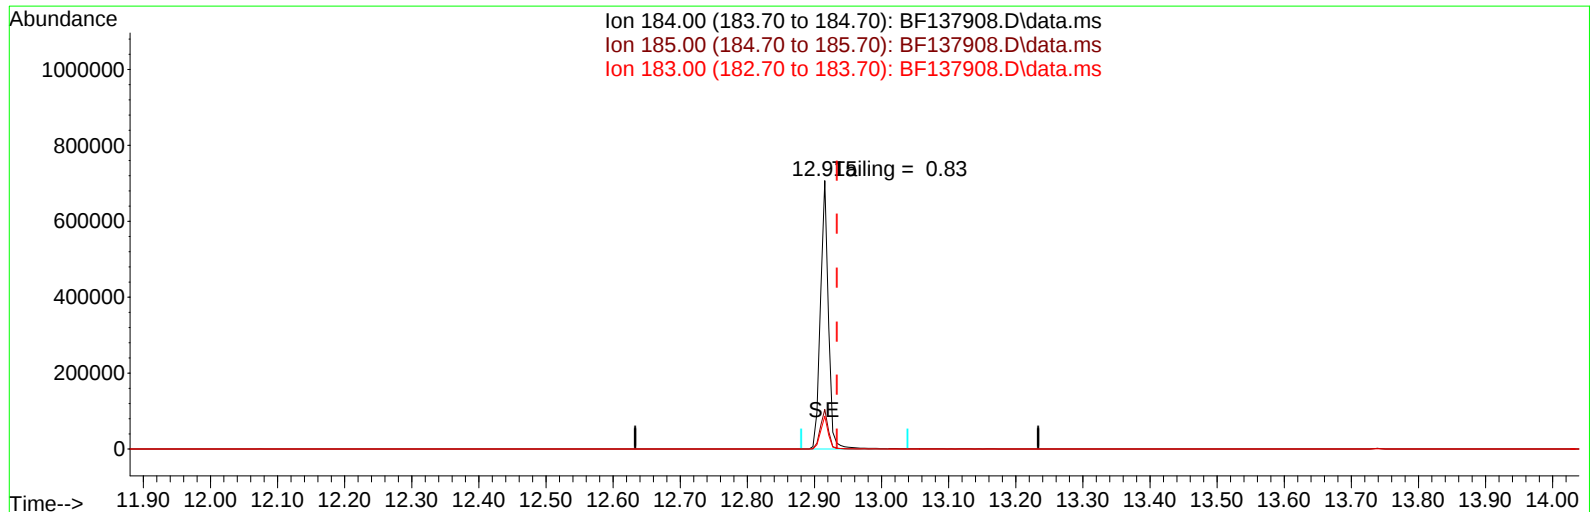

TIC: BF137908.D\data.ms

(77) Benzidine

12.915min (-0.018) 0.00 ng m

response 584349

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.72
183.00	11.50	12.24
0.00	0.00	0.00