


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051424\
Data File : BF137908.D
Acq On : 14 May 2024 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

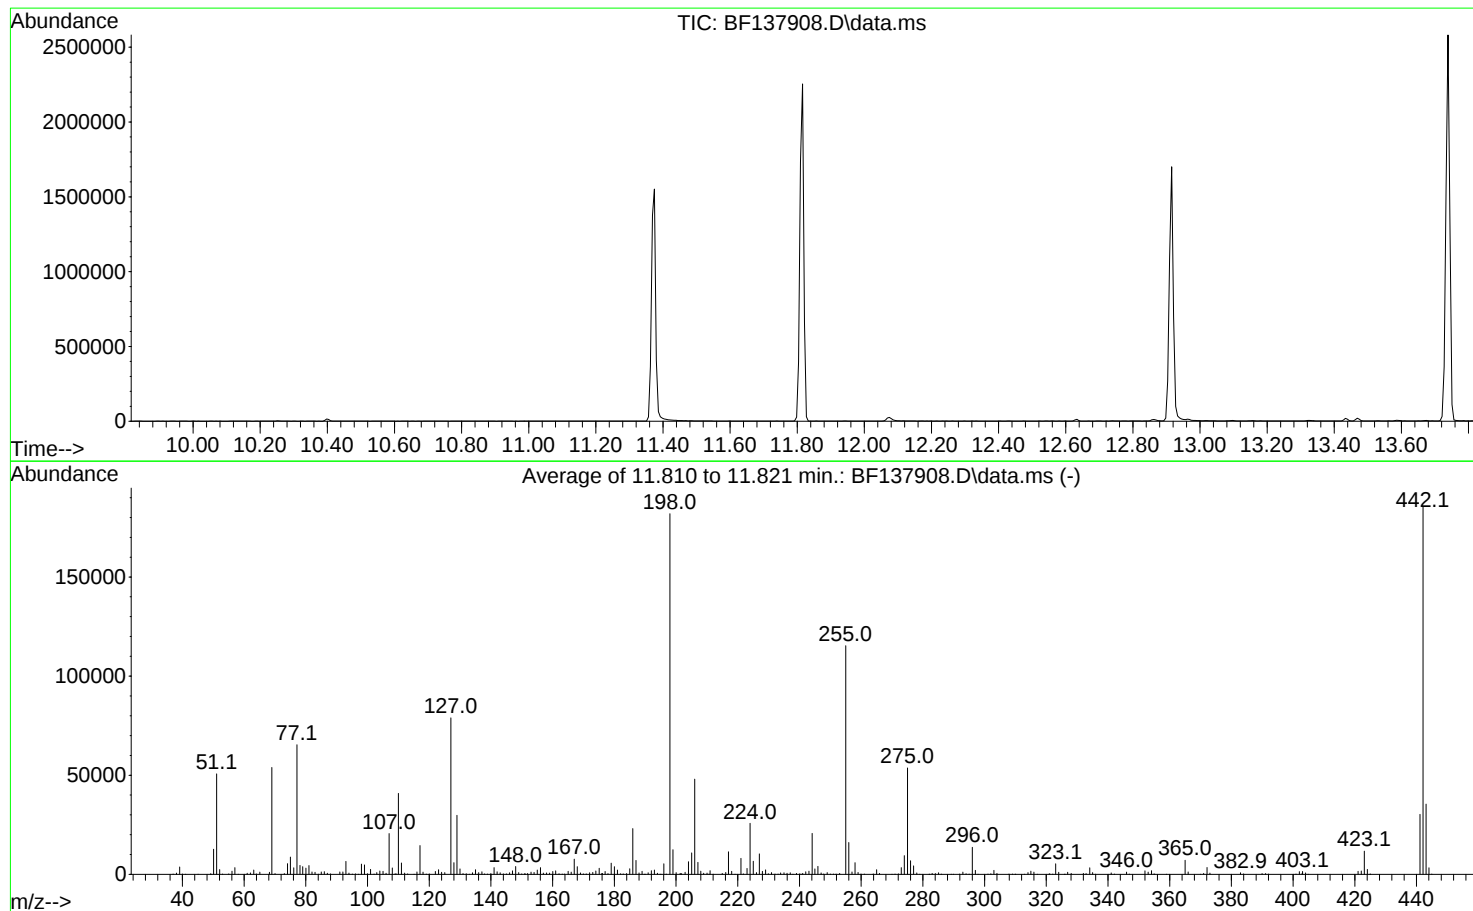




AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1647

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	50679	PASS
68	69	0.00	2	1.9	1042	PASS
69	198	0.00	100	29.6	53910	PASS
70	69	0.00	2	0.8	413	PASS
127	198	10	80	43.4	78901	PASS
197	198	0.00	2	0.1	177	PASS
198	198	100	100	100.0	181893	PASS
199	198	5	9	6.9	12475	PASS
275	198	10	60	29.5	53693	PASS
365	198	1	100	3.9	7072	PASS
441	198	0.01	100	16.7	30307	PASS
442	442	50	100	100.0	185560	PASS
443	442	15	24	19.1	35459	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051424\
Data File : BF137908.D
Acq On : 14 May 2024 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 14 12:38:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

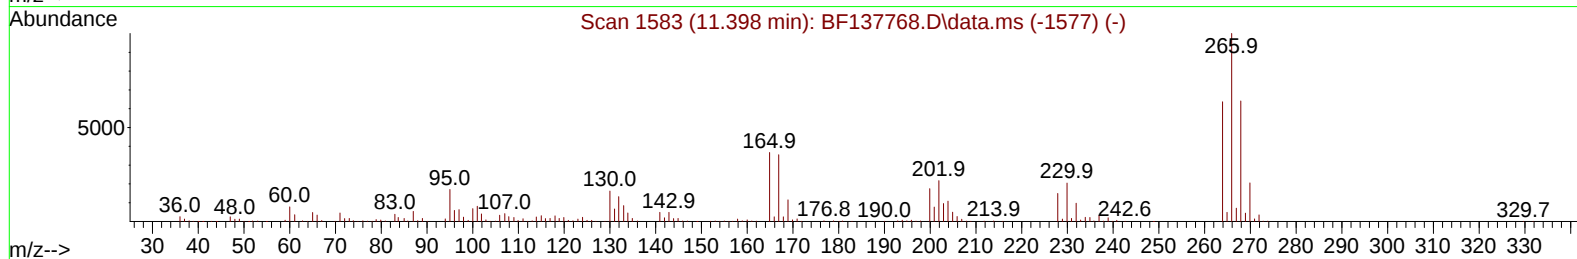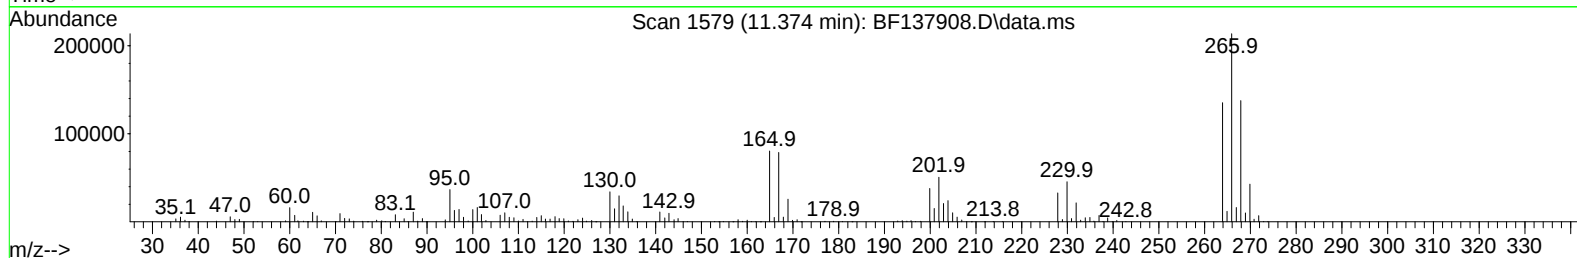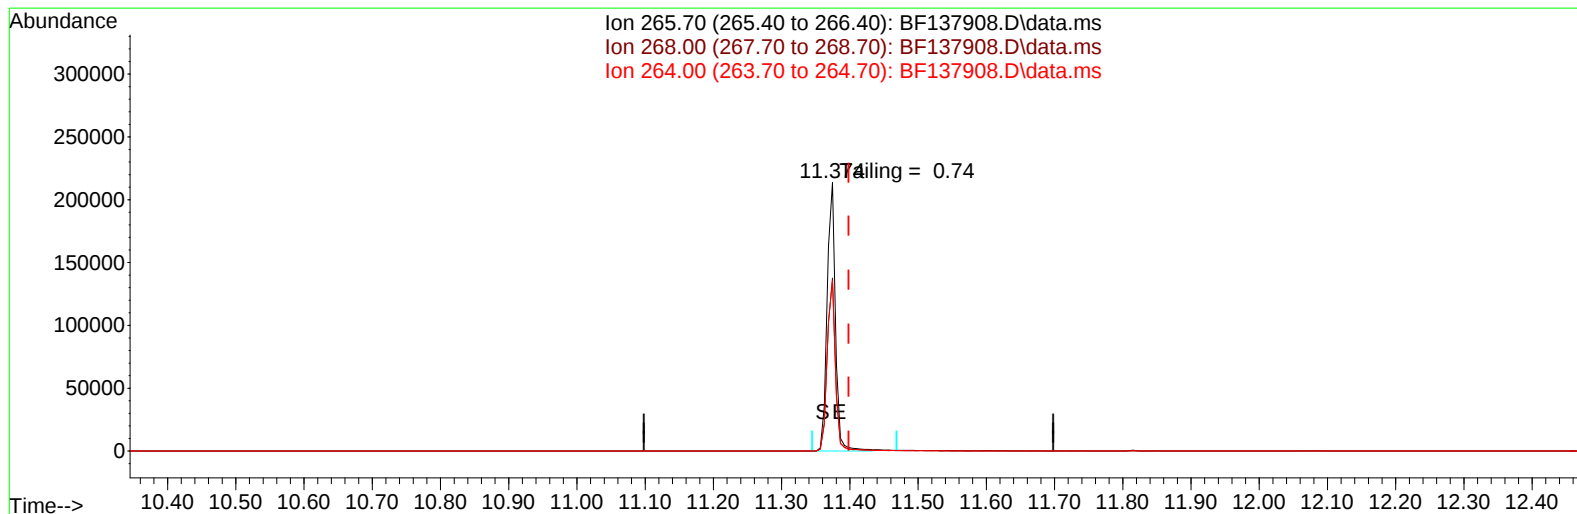

TIC: BF137908.D\data.ms

(70) Pentachlorophenol (C)

11.374min (-0.024) 27547.94 ng




response 181379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.44
264.00	63.70	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051424\
Data File : BF137908.D
Acq On : 14 May 2024 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 14 12:38:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

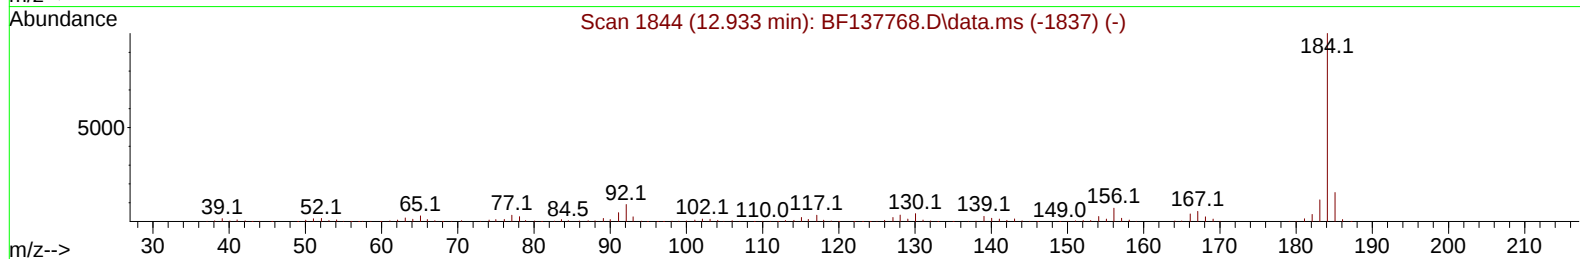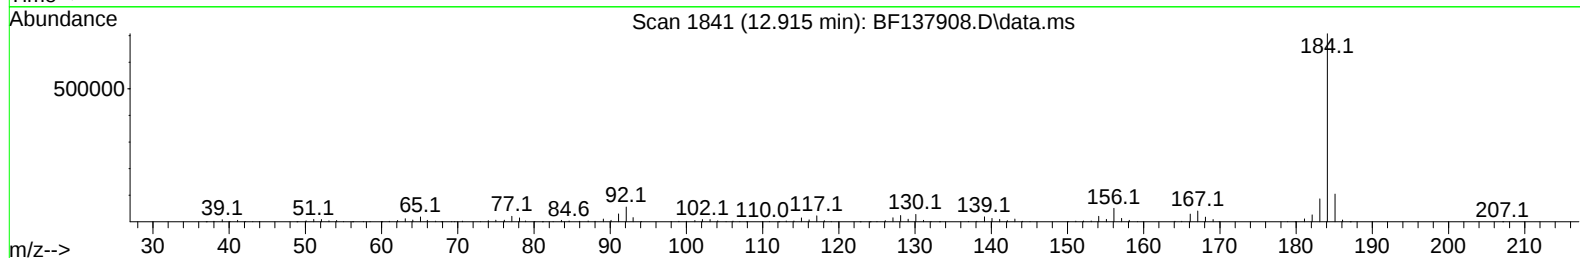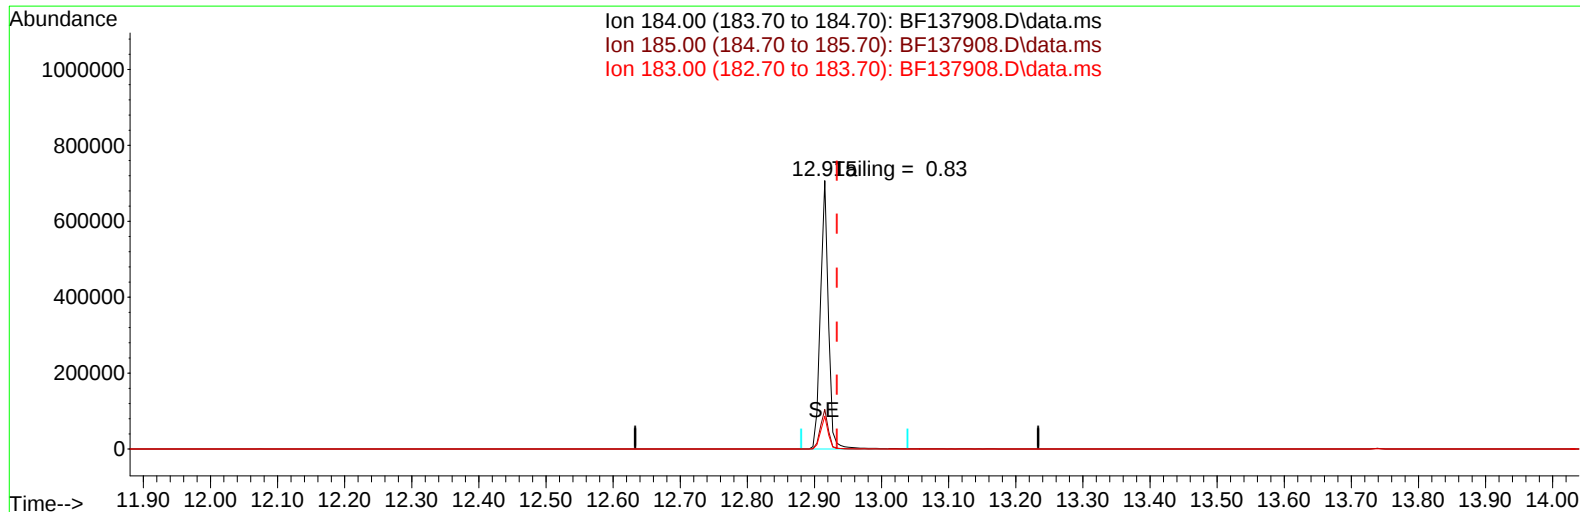

TIC: BF137908.D\data.ms

(77) Benzidine

12.915min (-0.018) 0.00 ng m

response 584349

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.72
183.00	11.50	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/14/2024	BNA_F	<u>BF137908.D</u>
Compound Name	Response	Retention Time
DDT	429306	13.739
DDD	6780	13.433
DDE	651	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7431	436737	1.70

Instrument :
BNA_F
ClientSampleId :
DFTPP