

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051515\
 Data File : BF079267.D
 Acq On : 15 May 2015 13:58
 Operator : TP/IZ
 Sample : PB83401BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB83401BL

Quant Time: May 15 23:15:16 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 15 22:54:46 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.18	152	54756	20.00	ng	0.00
21) Naphthalene-d8	8.75	136	232742	20.00	ng	0.00
38) Acenaphthene-d10	10.92	164	112429	20.00	ng	0.00
63) Phenanthrene-d10	12.76	188	217398	20.00	ng	0.00
75) Chrysene-d12	16.07	240	205766	20.00	ng	-0.02
86) Perylene-d12	17.86	264	195998	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	54447	17.12	ng	0.00
7) Phenol-d6	6.74	99	76857	18.28	ng	-0.01
23) Nitrobenzene-d5	7.87	82	38743	9.57	ng	0.00
41) 2,4,6-Tribromophenol	11.91	330	18444	15.16	ng	0.00
44) 2-Fluorobiphenyl	10.10	172	92762	11.49	ng	0.00
78) Terphenyl-d14	14.77	244	101827	11.85	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051515\
Data File : BF079267.D
Acq On : 15 May 2015 13:58
Operator : TP/IZ
Sample : PB83401BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB83401BL

Quant Time: May 15 23:15:16 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 15 22:54:46 2015
Response via : Initial Calibration




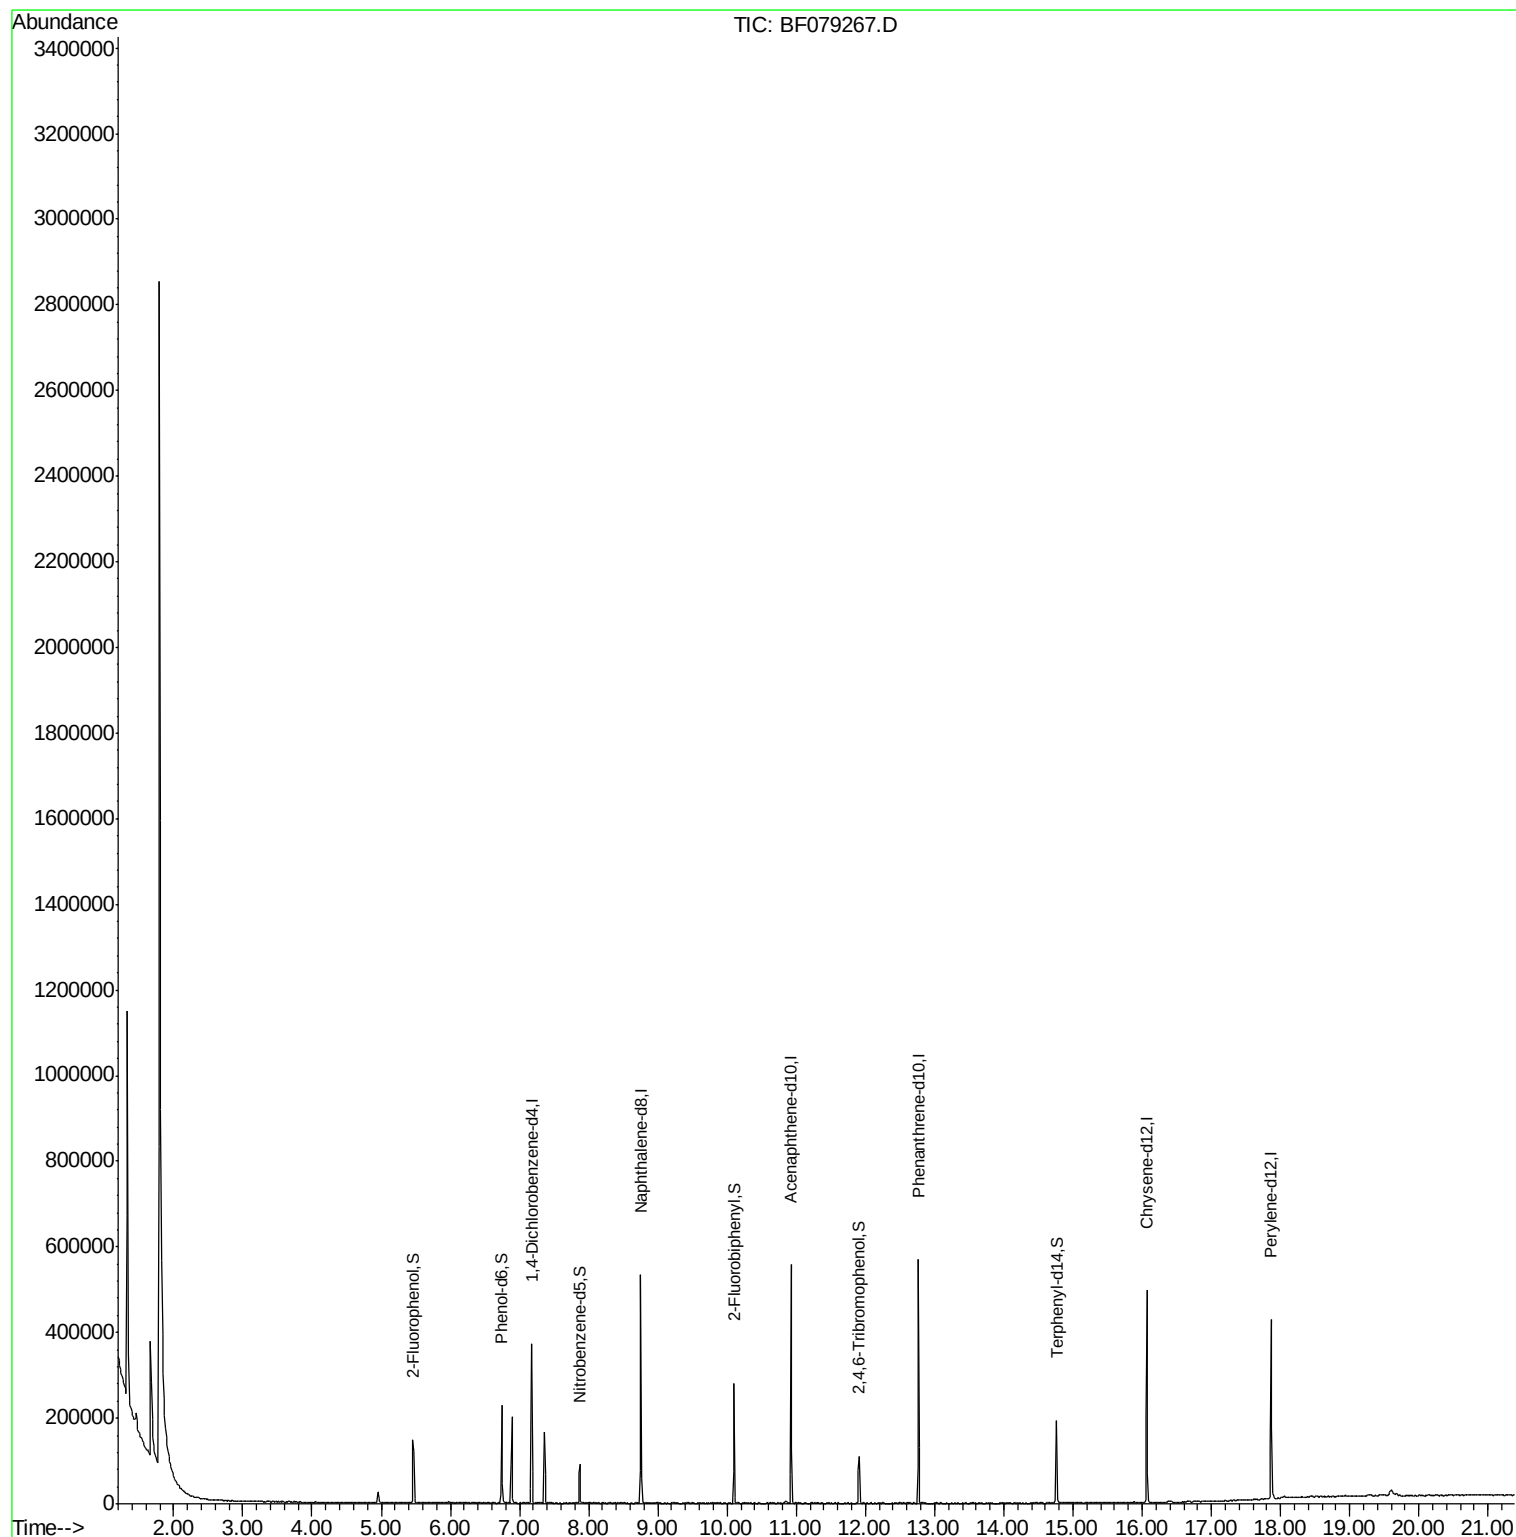


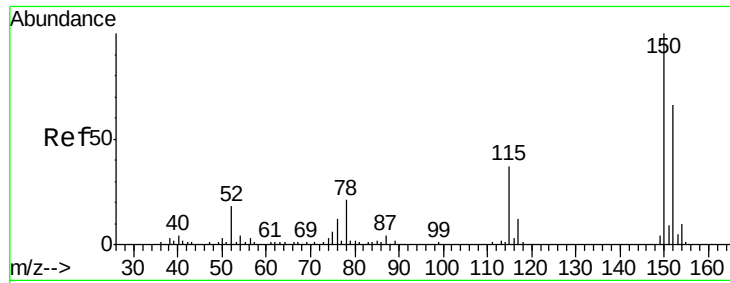

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.18 min Scan# 524
 Delta R.T. -0.00 min
 Lab File: BF079267.D
 Acq: 15 May 2015 13:58




Instrument :
 BNA_F
 ClientSampleId :
 PB83401BL


Tgt Ion:152 Resp: 54756
 Ion Ratio Lower Upper
 152 100
 150 160.1 123.8 185.8
 115 63.2 49.4 74.0

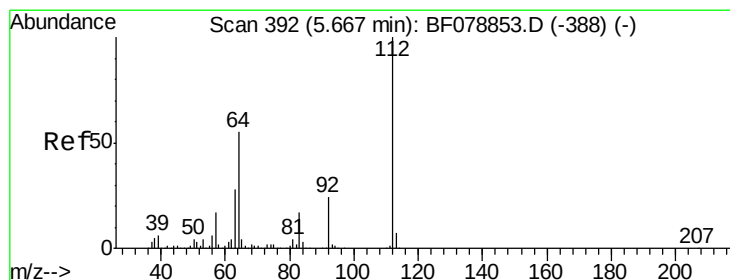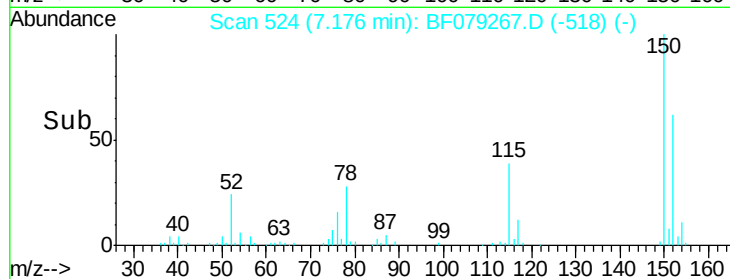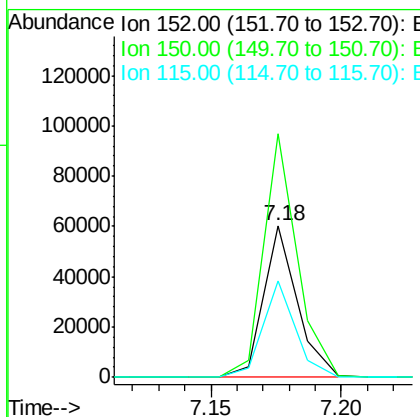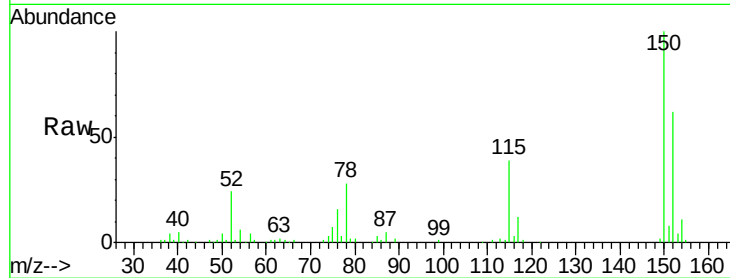

#5
 2-Fluorophenol
 Concen: 17.12 ng
 RT: 5.46 min Scan# 374
 Delta R.T. -0.00 min
 Lab File: BF079267.D
 Acq: 15 May 2015 13:58

Tgt Ion:112 Resp: 54447
 Ion Ratio Lower Upper
 112 100
 64 69.0 44.2 66.2#
 63 33.5 22.7 34.1

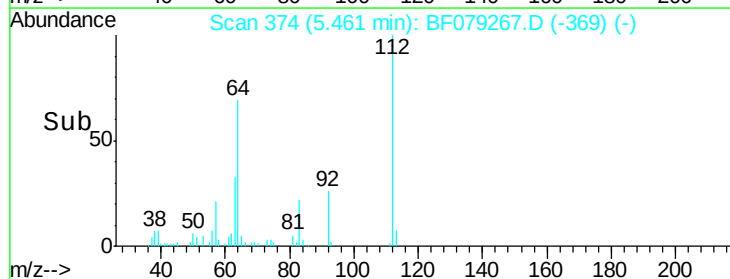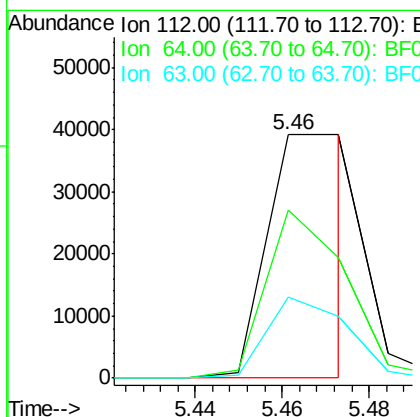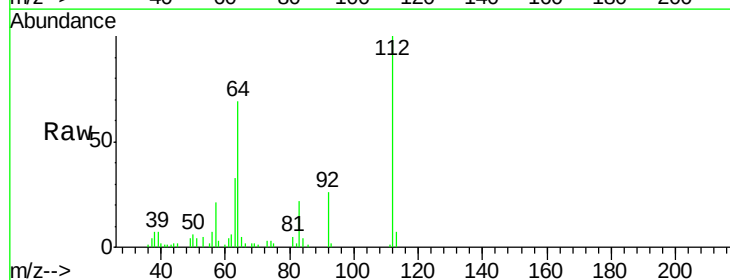

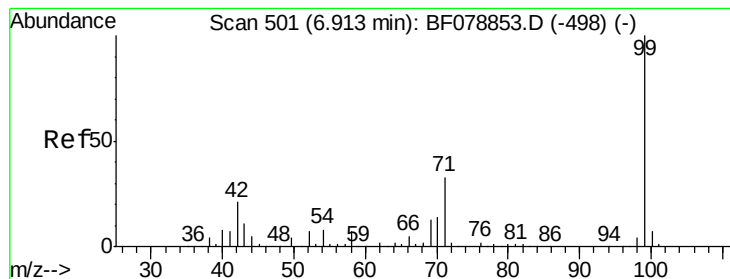

#7

Phenol-d6

Concen: 18.28 ng

RT: 6.74 min Scan# 486

Delta R.T. -0.01 min

Lab File: BF079267.D

Acq: 15 May 2015 13:58

Instrument :

BNA_F

ClientSampleId :

PB83401BL


Tgt Ion: 99 Resp: 76857

Ion Ratio Lower Upper

99 100

42 19.4 17.1 25.7




71 30.5 26.3 39.5

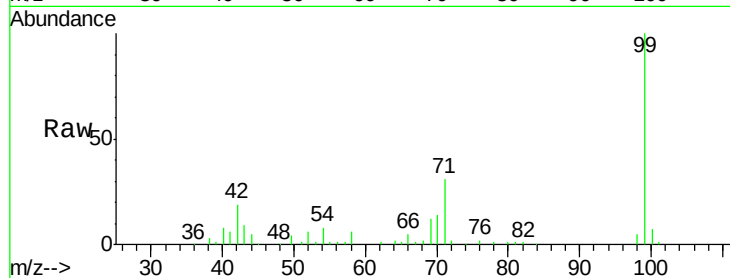

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

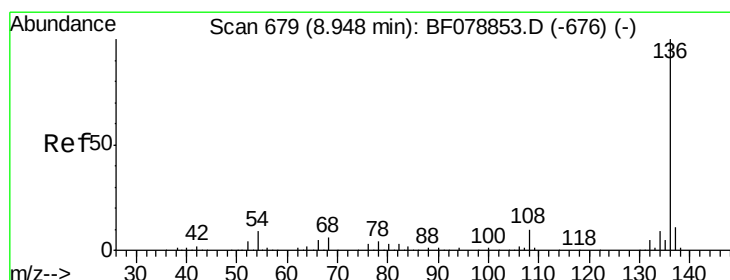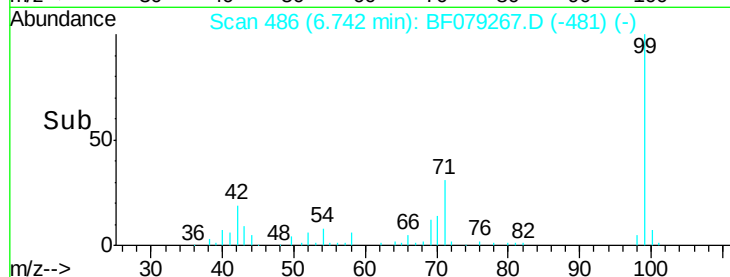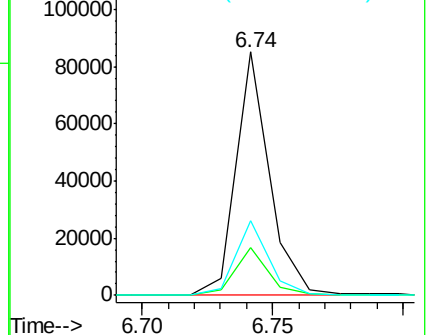

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.75 min Scan# 662

Delta R.T. -0.00 min

Lab File: BF079267.D

Acq: 15 May 2015 13:58

Tgt Ion: 136 Resp: 232742


Ion Ratio Lower Upper

136 100

137 10.7 8.8 13.2

54 7.5 6.9 10.3

68 5.5 4.9 7.3


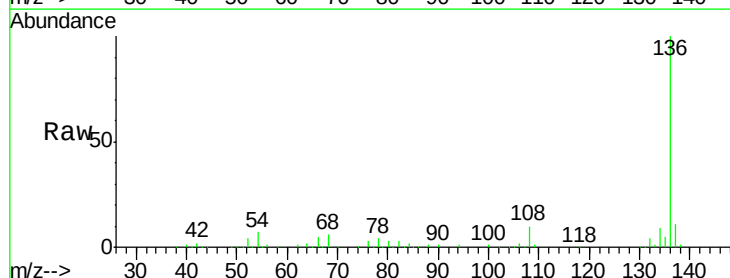



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

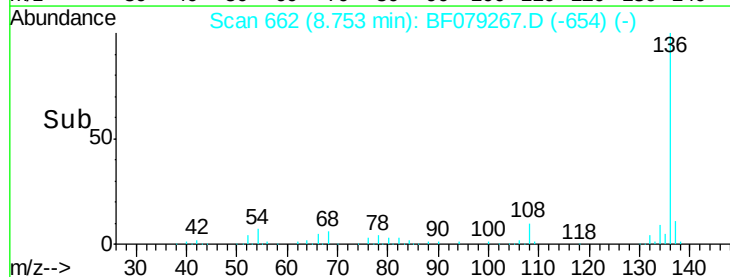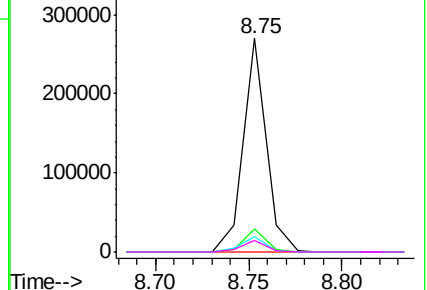


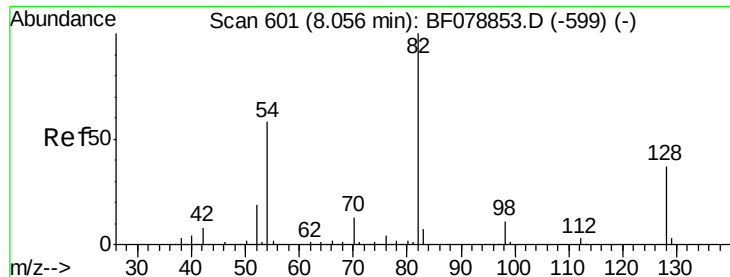




#23
 Nitrobenzene-d5
 Concen: 9.57 ng
 RT: 7.87 min Scan# 585
 Delta R.T. -0.00 min
 Lab File: BF079267.D
 Acq: 15 May 2015 13:58

Instrument :
 BNA_F
 ClientSampleID :
 PB83401BL

Tgt Ion: 82 Resp: 38743
 Ion Ratio Lower Upper
 82 100
 128 51.6 29.7 44.5#
 54 48.8 46.2 69.4

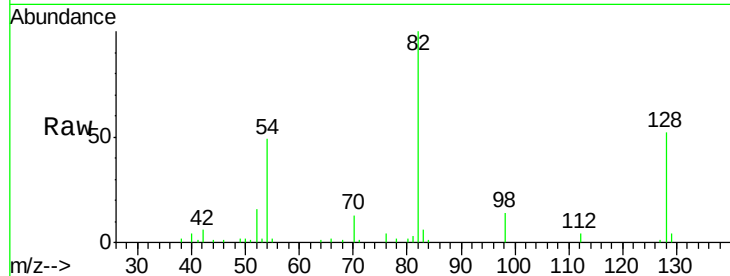


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

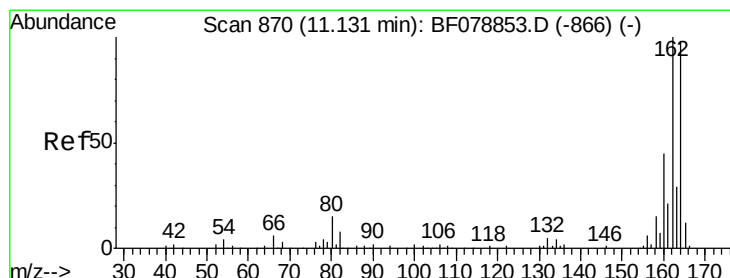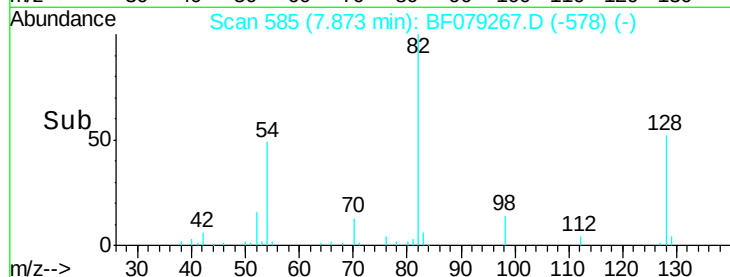
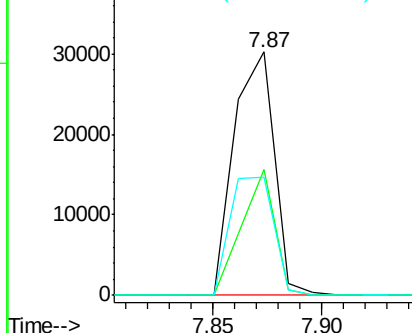



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.92 min Scan# 852
 Delta R.T. -0.00 min
 Lab File: BF079267.D
 Acq: 15 May 2015 13:58

Tgt Ion: 164 Resp: 112429
 Ion Ratio Lower Upper
 164 100
 162 101.2 81.4 122.0
 160 46.3 36.6 54.8

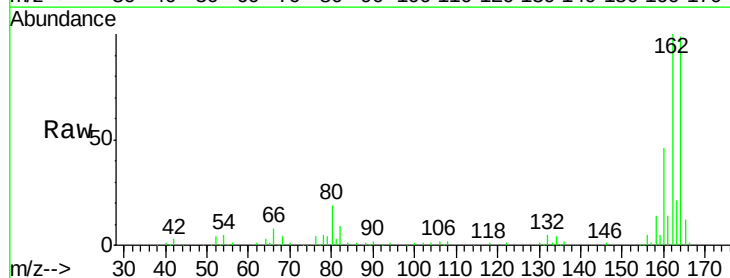

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

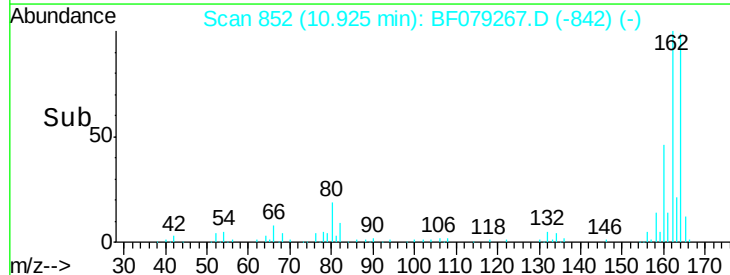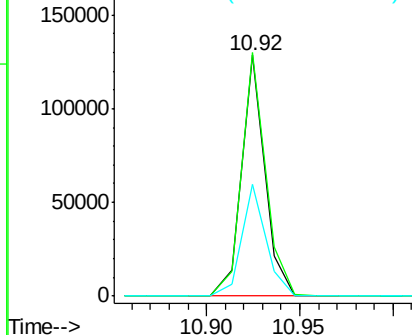


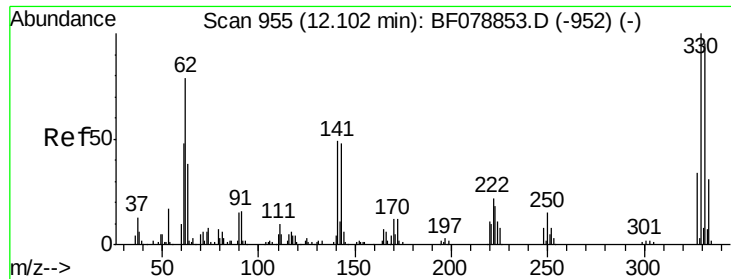




#41
 2,4,6-Tribromophenol
 Concen: 15.16 ng
 RT: 11.91 min Scan# 938
 Delta R.T. -0.00 min
 Lab File: BF079267.D
 Acq: 15 May 2015 13:58

Instrument :
 BNA_F
 ClientSampleId :
 PB83401BL

Tgt Ion:330 Resp: 18444
 Ion Ratio Lower Upper
 330 100
 332 104.0 76.9 115.3
 141 33.8 27.8 41.8

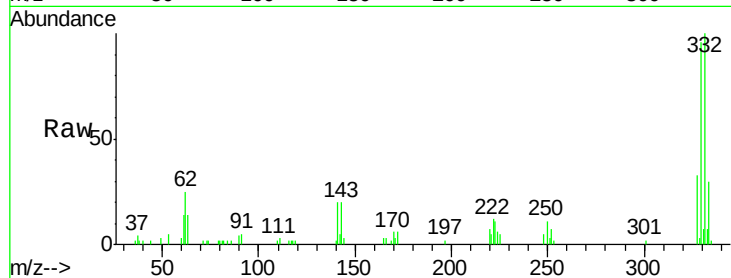


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

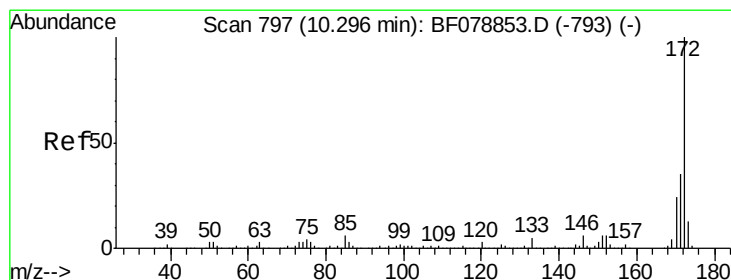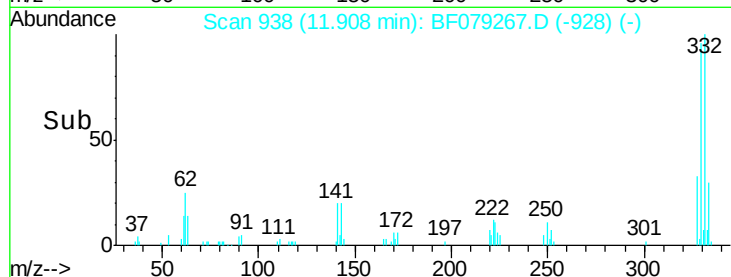
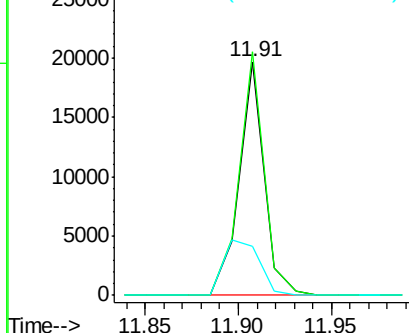



#44
 2-Fluorobiphenyl
 Concen: 11.49 ng
 RT: 10.10 min Scan# 780
 Delta R.T. -0.00 min
 Lab File: BF079267.D
 Acq: 15 May 2015 13:58

Tgt Ion:172 Resp: 92762
 Ion Ratio Lower Upper
 172 100
 171 34.5 28.3 42.5
 170 23.0 19.4 29.2

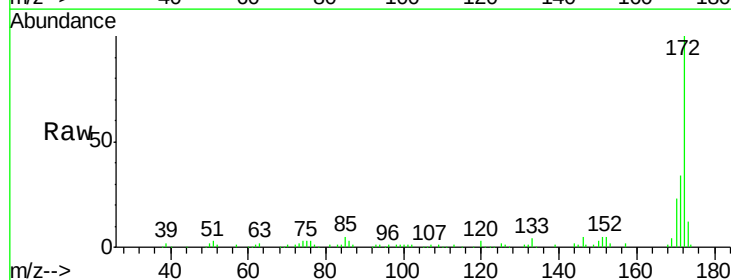

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

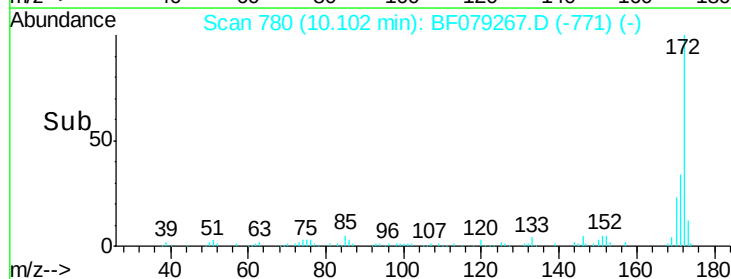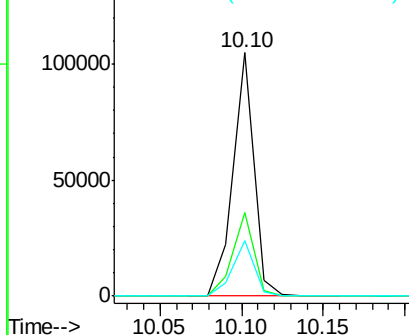


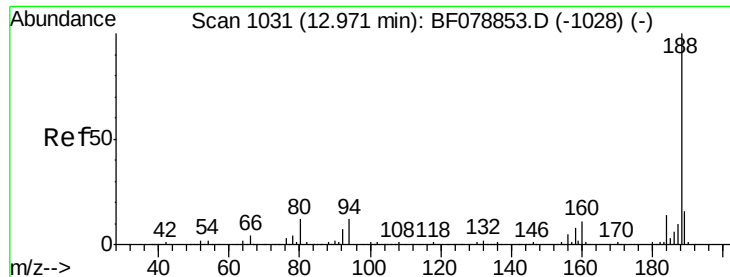




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.76 min Scan# 1013
Delta R.T. -0.00 min
Lab File: BF079267.D
Acq: 15 May 2015 13:58

Instrument :
BNA_F
ClientSampleId :
PB83401BL

Tgt Ion:188 Resp: 217398
Ion Ratio Lower Upper
188 100
94 10.2 9.4 14.0
80 10.7 9.8 14.6

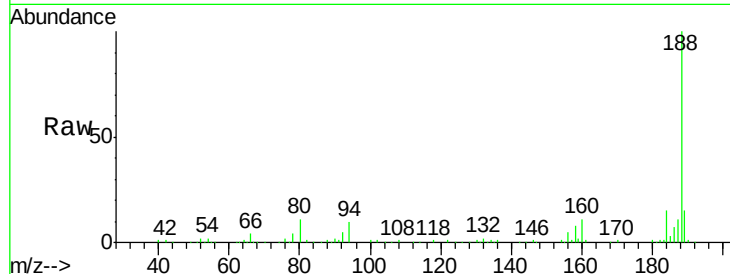


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

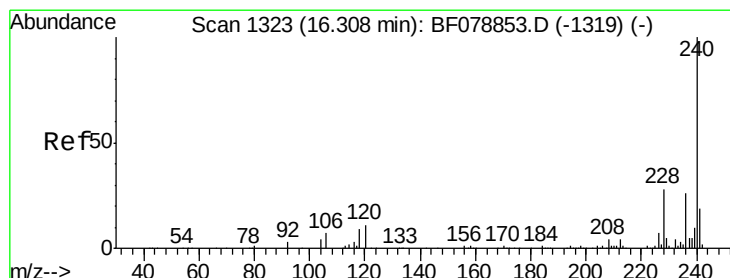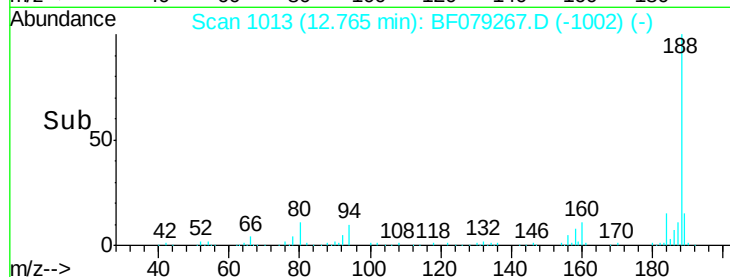
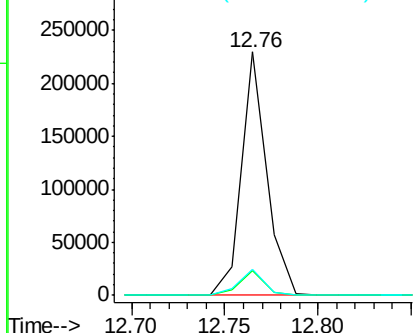



#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.07 min Scan# 1302
Delta R.T. -0.02 min
Lab File: BF079267.D
Acq: 15 May 2015 13:58

Tgt Ion:240 Resp: 205766
Ion Ratio Lower Upper
240 100
120 10.6 8.6 12.8
236 26.1 21.0 31.6

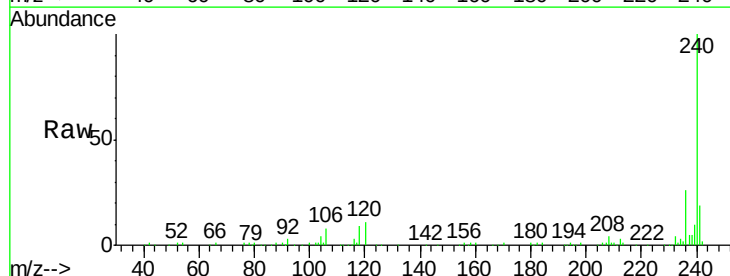

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

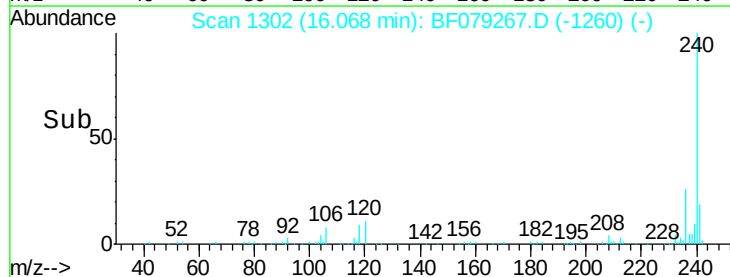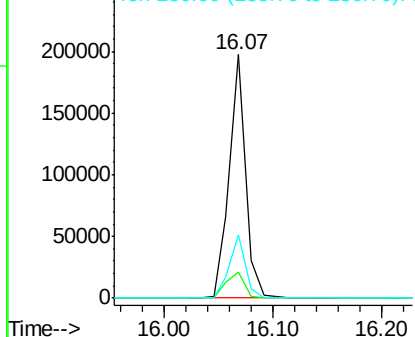

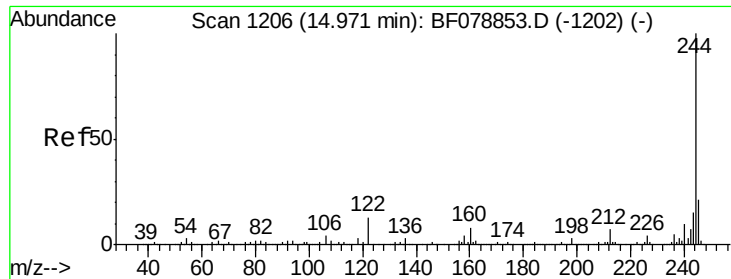

#78

Terphenyl-d14

Concen: 11.85 ng

RT: 14.77 min Scan# 1188

Delta R.T. -0.00 min

Lab File: BF079267.D

Acq: 15 May 2015 13:58

Instrument :

BNA_F

ClientSampleId :

PB83401BL


Tgt Ion:244 Resp: 101827

Ion Ratio Lower Upper

244 100

212 5.7 5.6 8.4




122 7.9 10.5 15.7#

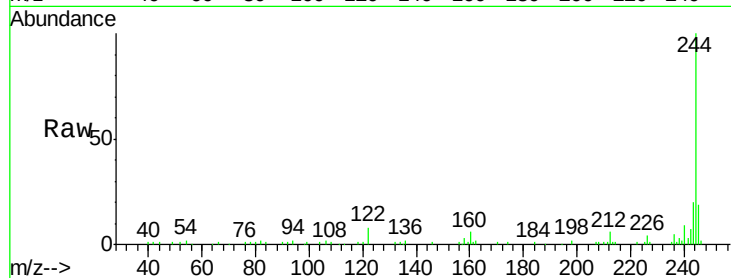

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

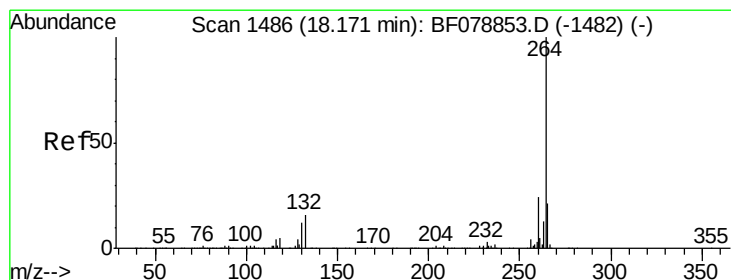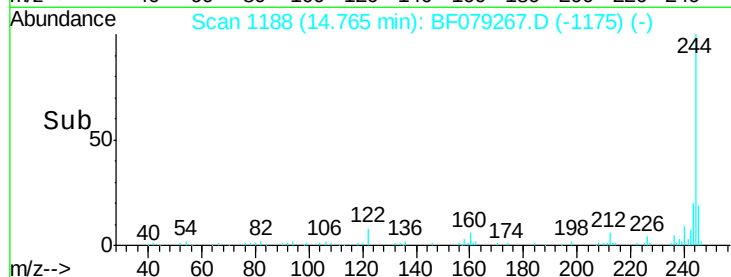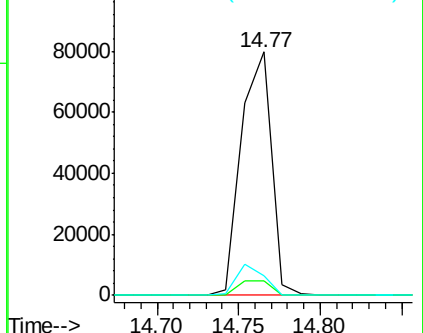

#86

Perylene-d12

Concen: 20.00 ng

RT: 17.86 min Scan# 1459

Delta R.T. -0.07 min

Lab File: BF079267.D

Acq: 15 May 2015 13:58


Tgt Ion:264 Resp: 195998

Ion Ratio Lower Upper

264 100

260 24.4 19.2 28.8

265 22.0 17.2 25.8

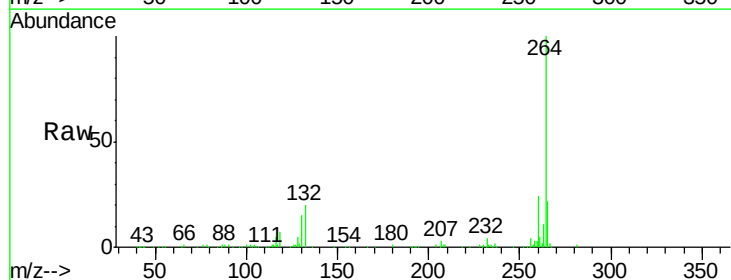

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

