


Data Path : Z:\HPCHEM1\BNA_F\Data\BF051515\
 Data File : BF079265.D
 Acq On : 15 May 2015 12:02
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 15 01:57:52 2015

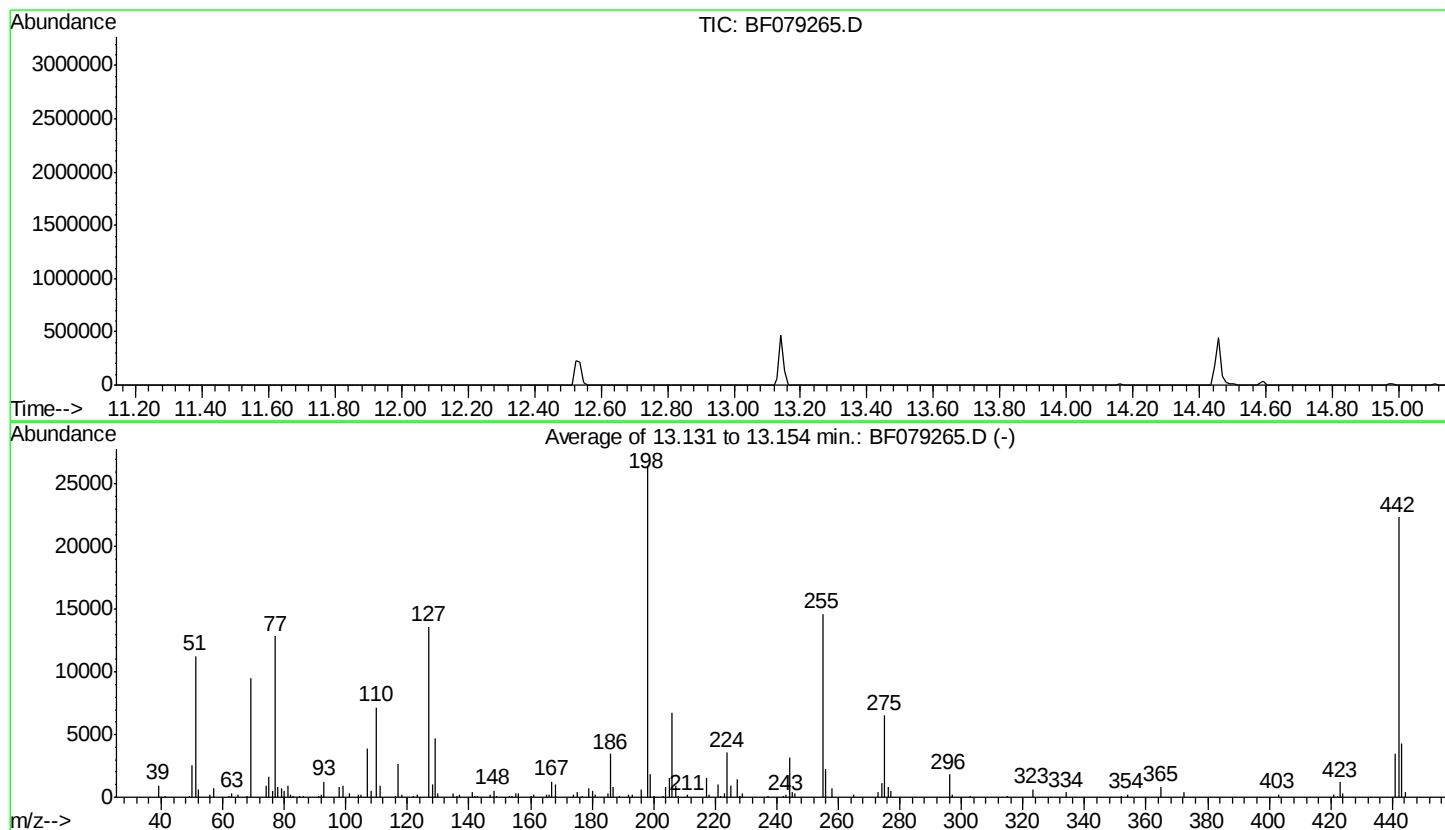

AutoFind: Scans 1045, 1046, 1047; Background Corrected with Scan 1042

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	11287	PASS
68	69	0.00	2	1.4	130	PASS
69	198	0.00	100	35.8	9473	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.4	13609	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26470	PASS
199	198	5	9	7.0	1865	PASS
275	198	10	60	24.6	6512	PASS
365	198	1	100	3.3	867	PASS
441	442	0.01	24	15.6	3486	PASS
442	198	50	100	84.4	22352	PASS
443	442	15	24	19.2	4285	PASS