


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051515\
Data File : BF079288.D
Acq On : 16 May 2015 1:36
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri May 15 22:54:46 2015

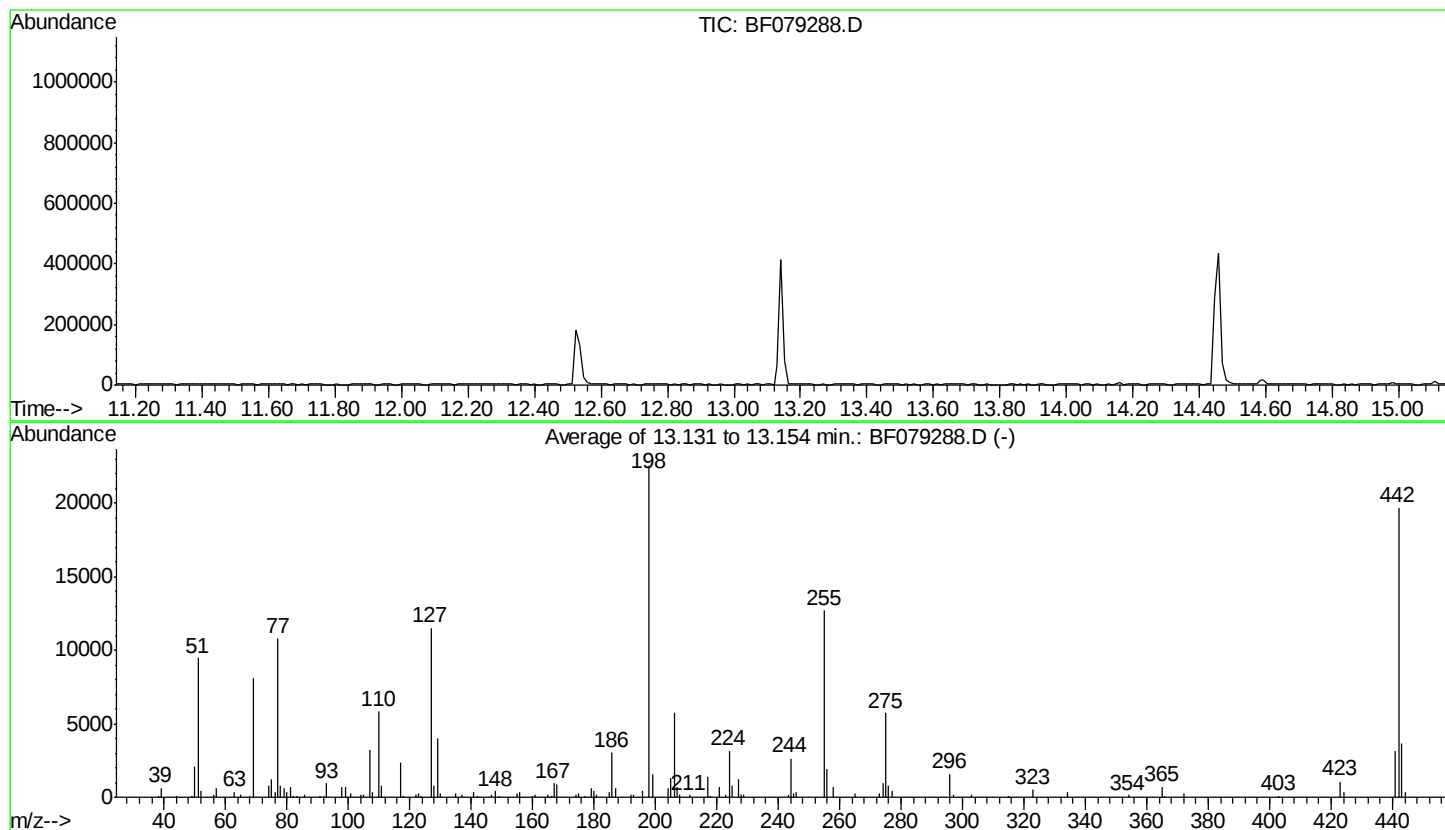

AutoFind: Scans 1045, 1046, 1047; Background Corrected with Scan 1042

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	9480	PASS
68	69	0.00	2	1.4	114	PASS
69	198	0.00	100	36.1	8130	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	11526	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22537	PASS
199	198	5	9	6.9	1565	PASS
275	198	10	60	25.4	5715	PASS
365	198	1	100	3.2	725	PASS
441	442	0.01	24	16.0	3152	PASS
442	198	50	100	87.3	19667	PASS
443	442	15	24	18.7	3682	PASS