


Data Path : Z:\HPCHEM1\BNA_G\Data\BG051515\
 Data File : BG017188.D
 Acq On : 15 May 2015 23:09
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG051315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 16:12:13 2015

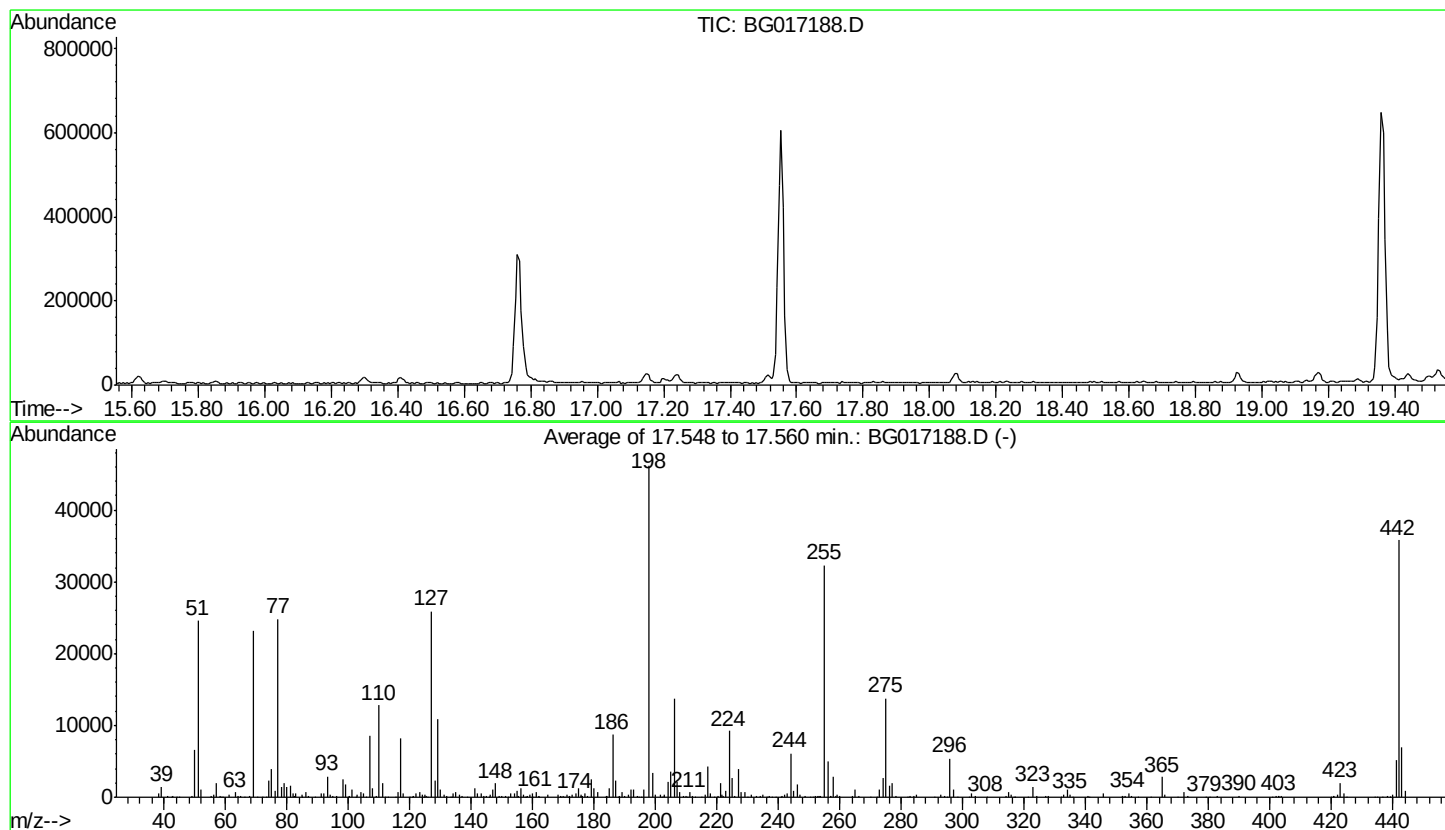

AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.2	24563	PASS
68	69	0.00	2	0.8	182	PASS
69	198	0.00	100	50.3	23240	PASS
70	69	0.00	2	0.2	55	PASS
127	198	10	80	56.2	25933	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46173	PASS
199	198	5	9	7.5	3444	PASS
275	198	10	60	29.7	13736	PASS
365	198	1	100	6.1	2817	PASS
441	442	0.01	24	14.5	5182	PASS
442	198	50	100	77.5	35773	PASS
443	442	15	24	19.4	6932	PASS