
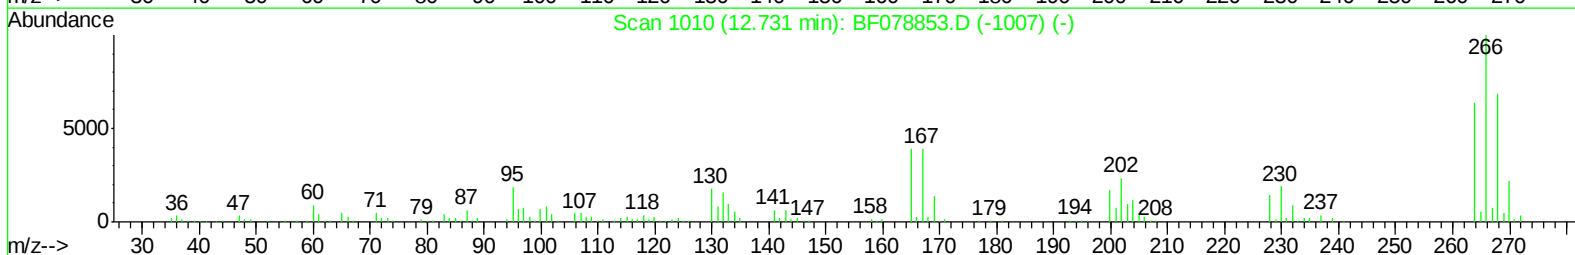
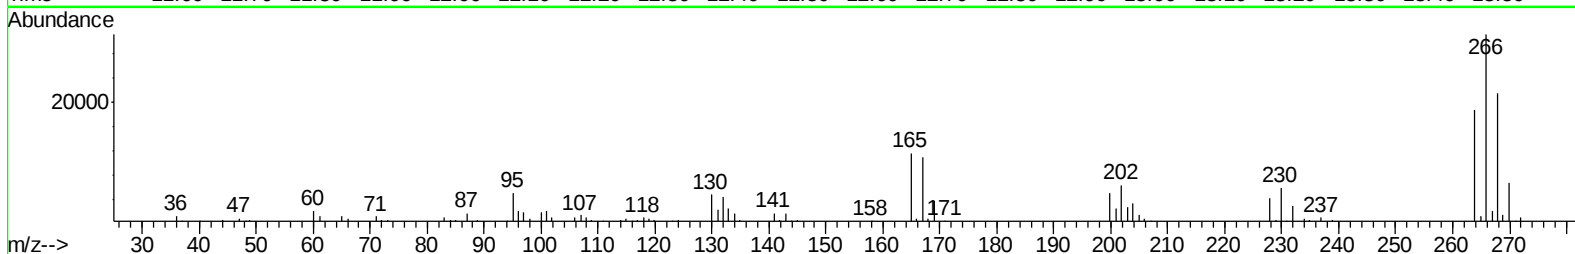


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051515\
Data File : BF079265.D
Acq On : 15 May 2015 12:02
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 03:25:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 18 00:56:30 2015
Response via : Initial Calibration

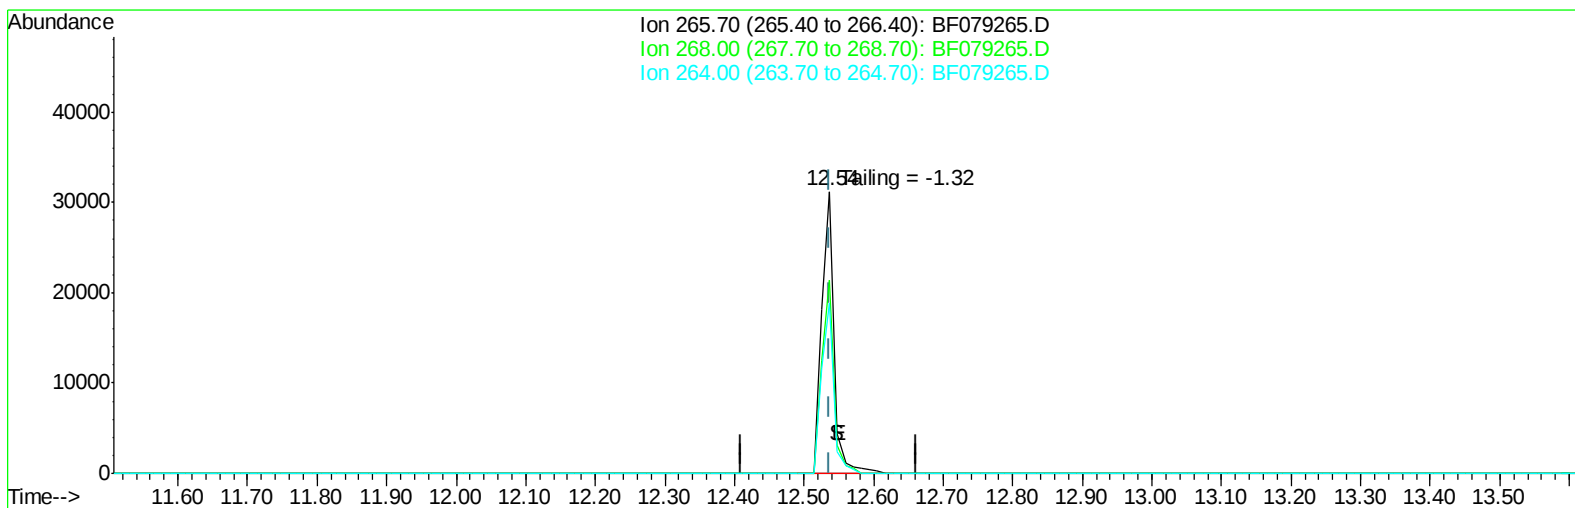

TIC: BF079265.D

(69) Pentachlorophenol (C)




12.536min (+0.000) 0.00ng m

response 38967

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	68.60
264.00	63.60	60.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051515\
Data File : BF079265.D
Acq On : 15 May 2015 12:02
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 03:25:48 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 18 00:56:30 2015
Response via : Initial Calibration

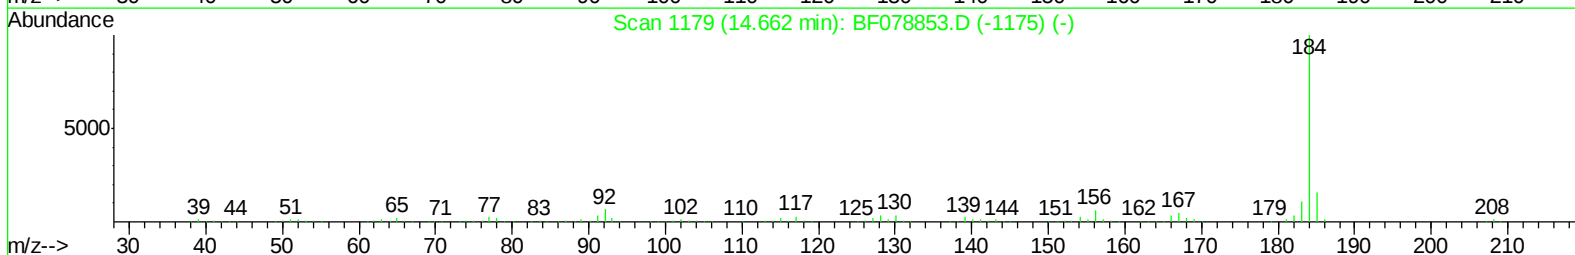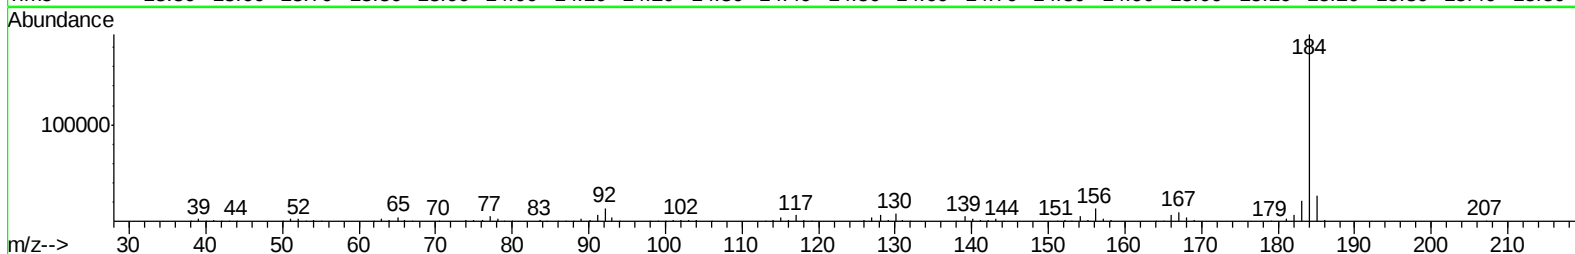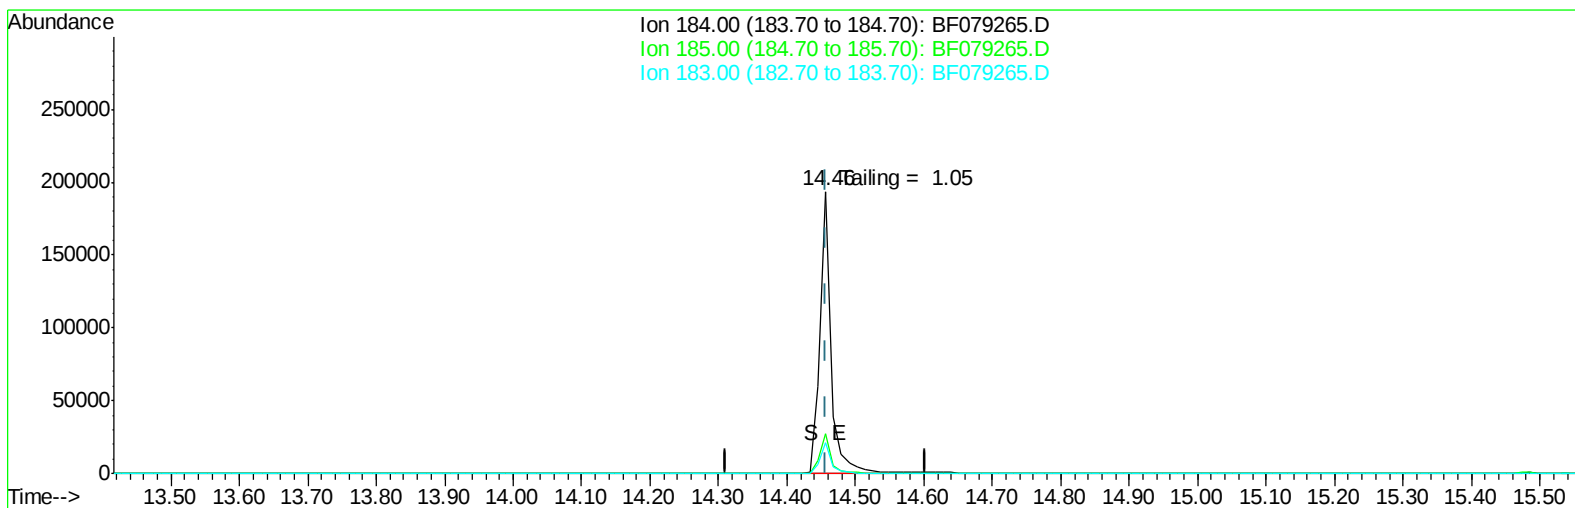

TIC: BF079265.D

(76) Benzidine

14.457min (+0.000) 0.00ng

response 222983

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.03
183.00	11.20	11.08
0.00	0.00	0.00