
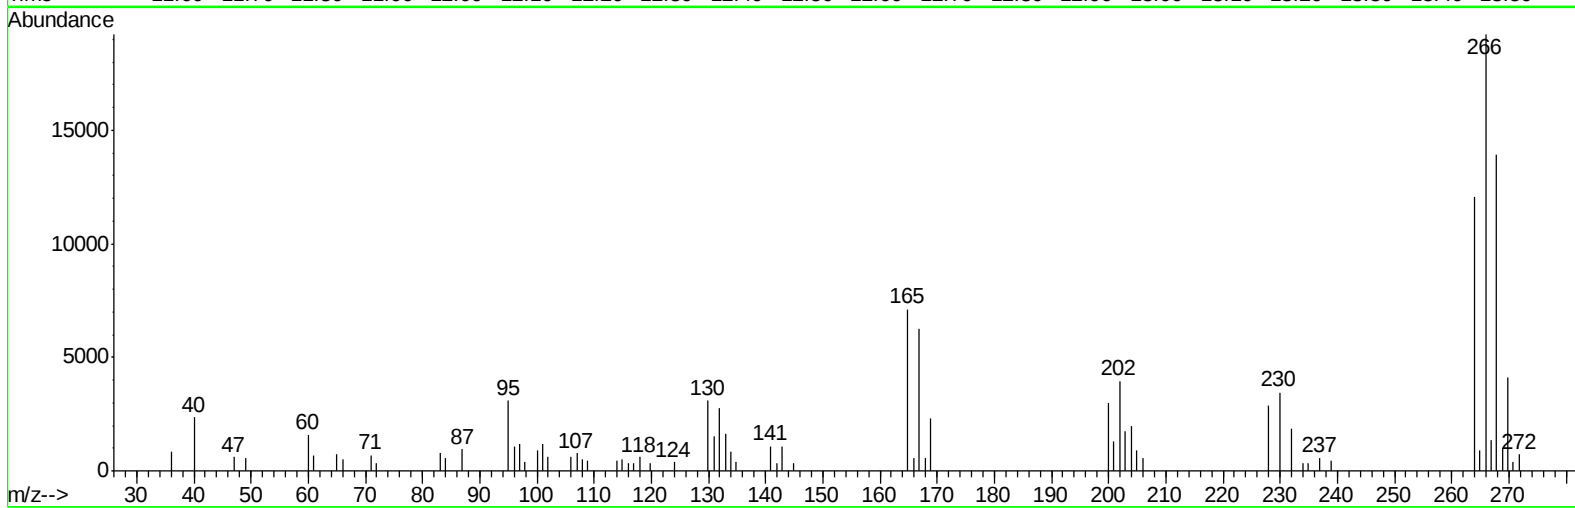


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051515\
Data File : BF079288.D
Acq On : 16 May 2015 1:36
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 18 03:27:18 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 18 00:56:30 2015
Response via : Initial Calibration

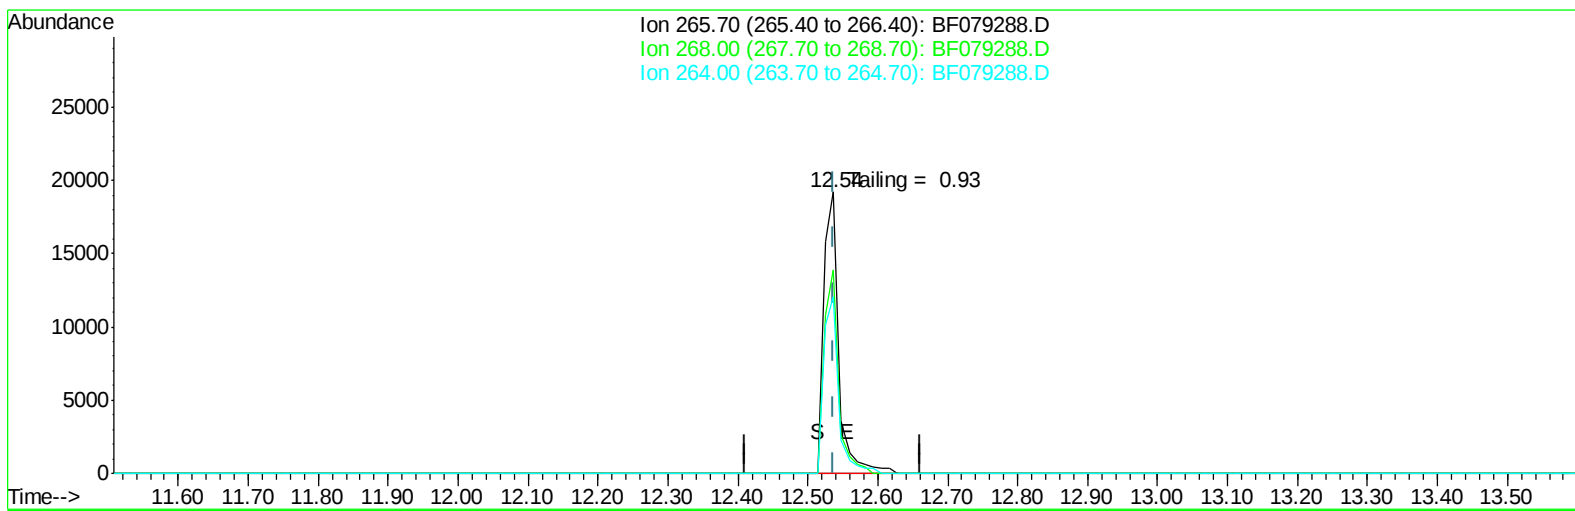

TIC: BF079288.D

(69) Pentachlorophenol (C)



12.536min (+0.000) 0.00ng

response 28937

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	72.36
264.00	63.60	62.83
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051515\  
Data File : BF079288.D  
Acq On    : 16 May 2015    1:36  
Operator  : TP/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 18 03:27:18 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 18 00:56:30 2015
Response via : Initial Calibration

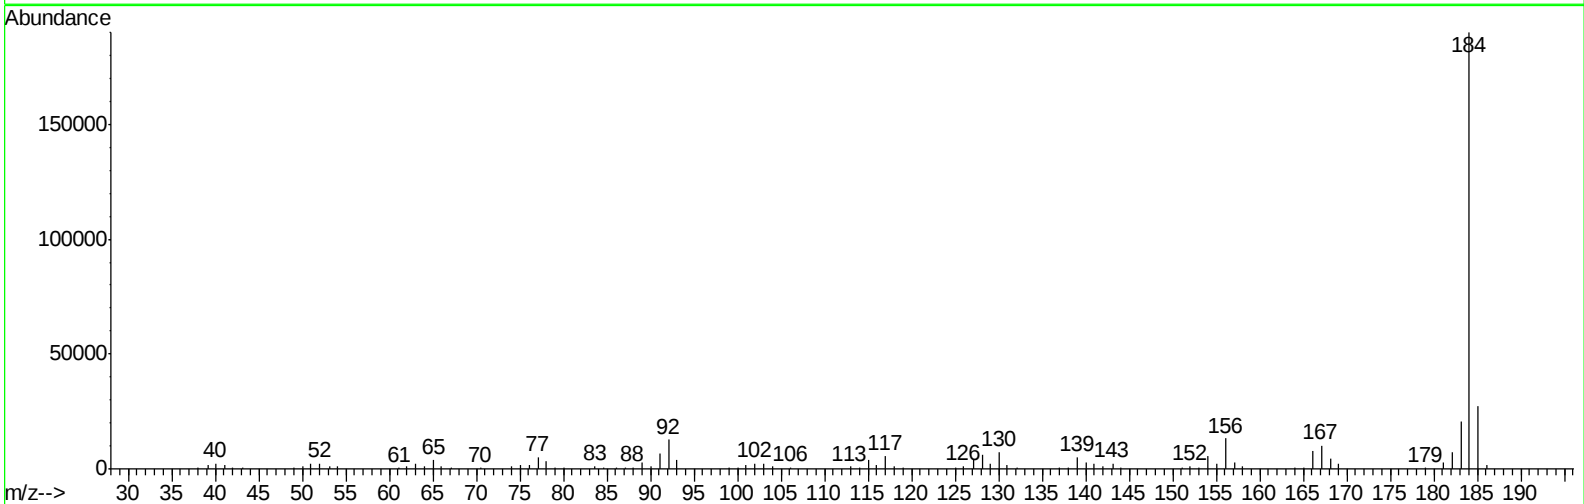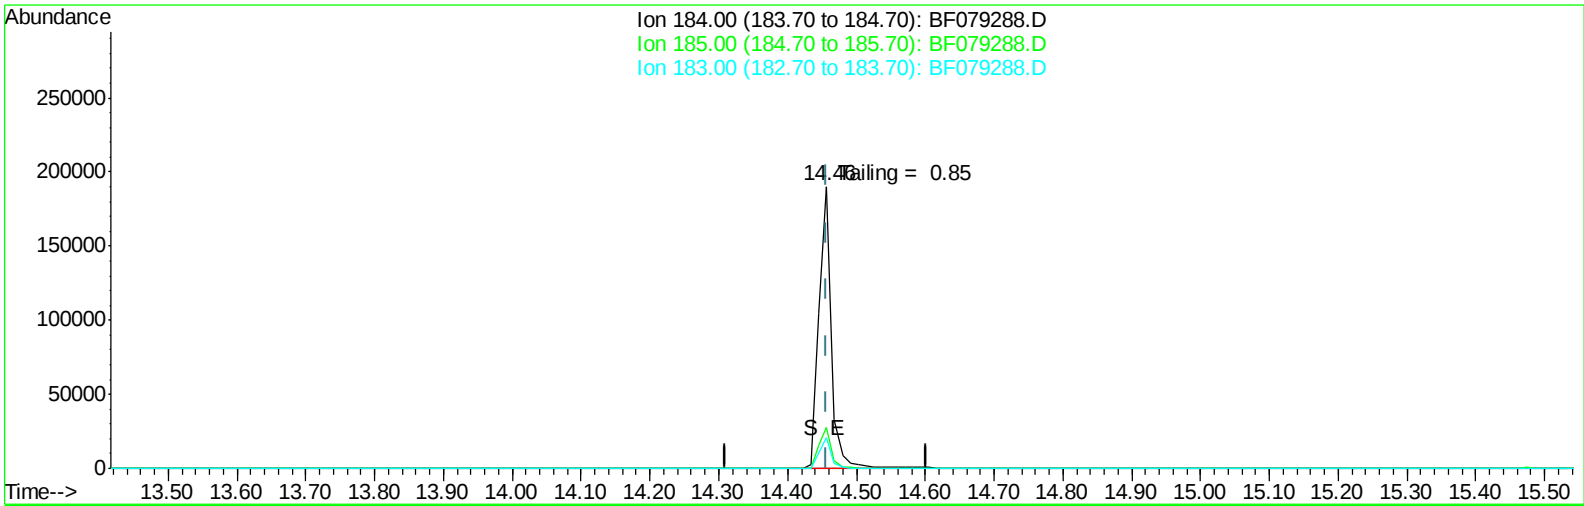

TIC: BF079288.D

(76) Benzidine

14.457min (+0.000) 0.00ng

response 239175

Ion	Exp%	Act%
184.00	100	100
185.00	16.00	14.50
183.00	11.20	10.90
0.00	0.00	0.00