
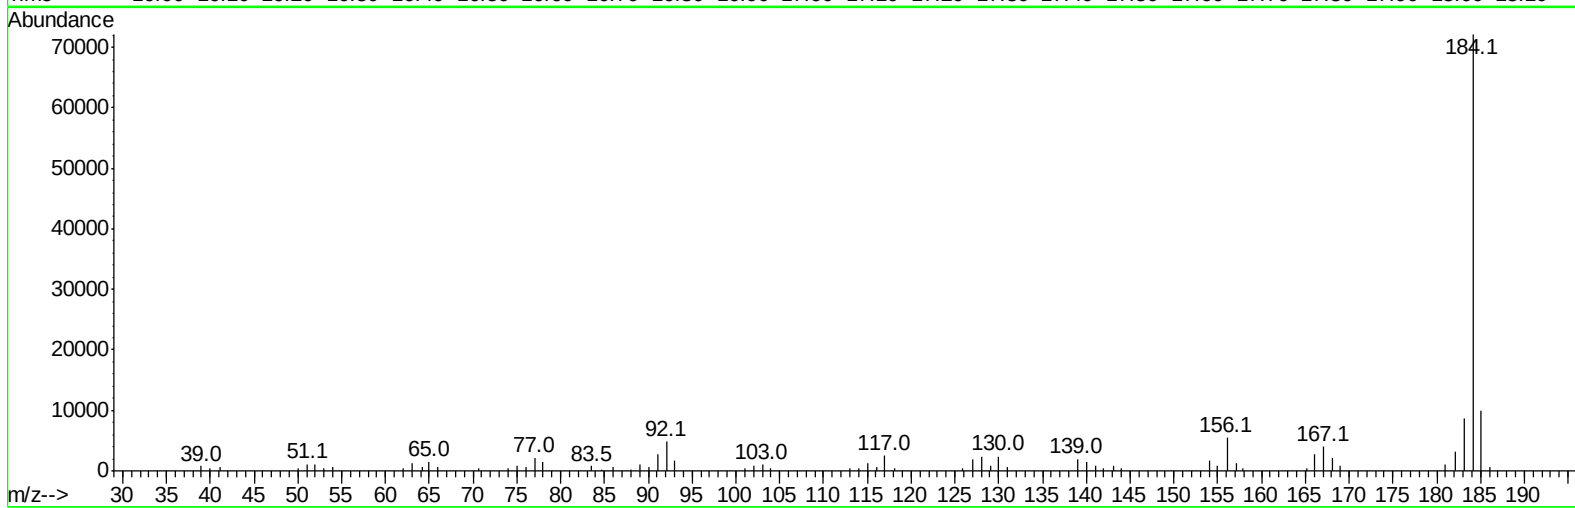


Data Path : Z:\HPCHEM1\BNA F\Data\BF051517\
Data File : BF095123.D
Acq On : 15 May 2017 13:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 00:48:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

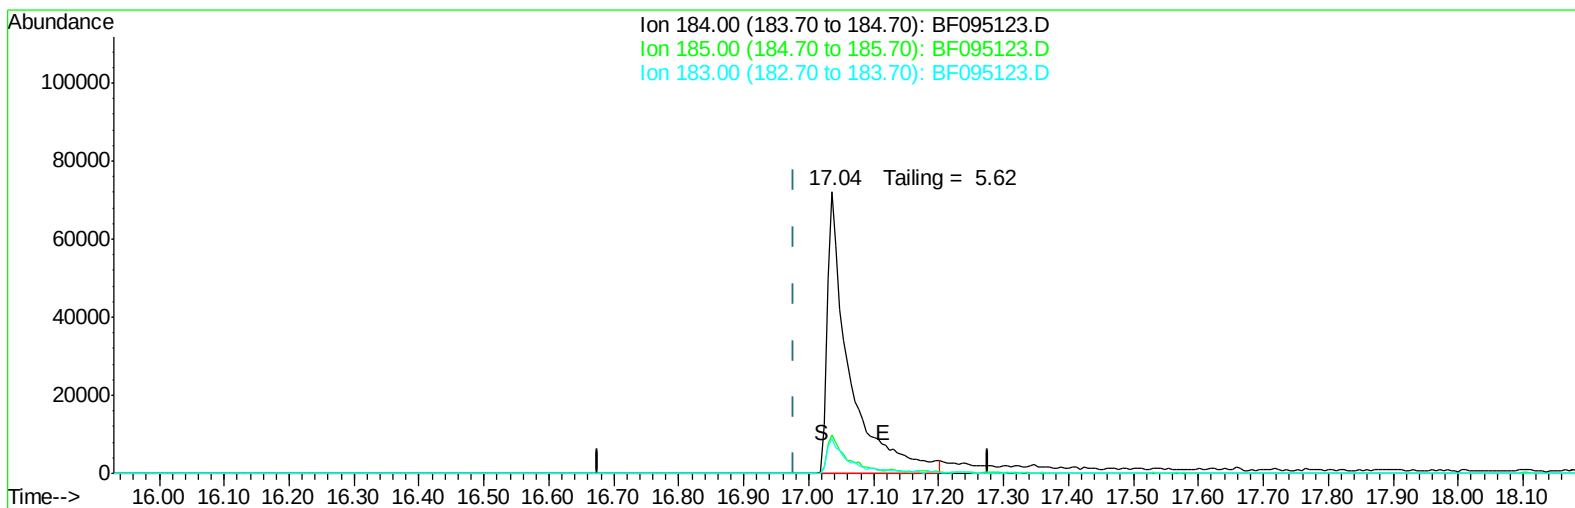

TIC: BF095123.D

(76) Benzidine




17.036min (+0.059) 0.00ng

response 166087

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.70#
183.00	12.20	12.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF051517\
Data File : BF095123.D
Acq On : 15 May 2017 13:41
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 17 00:48:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

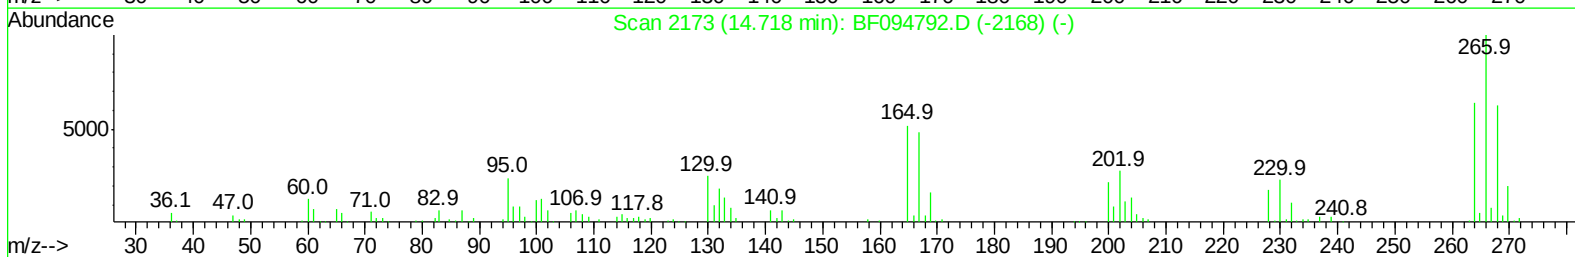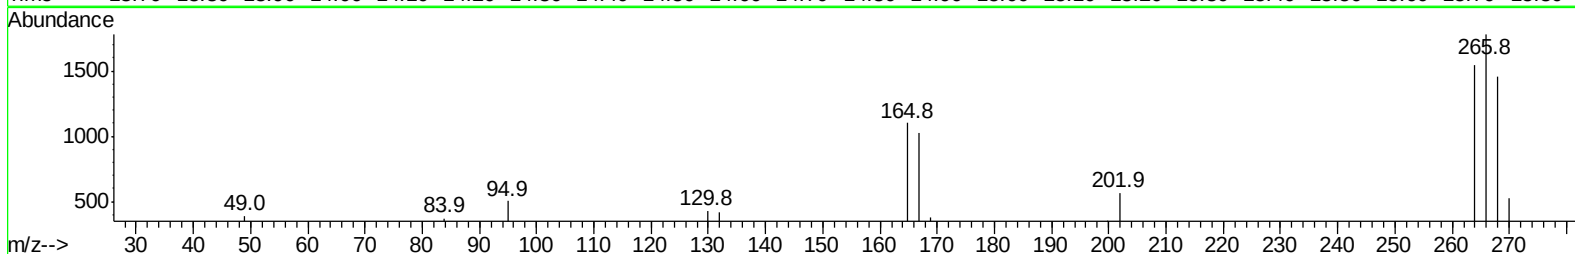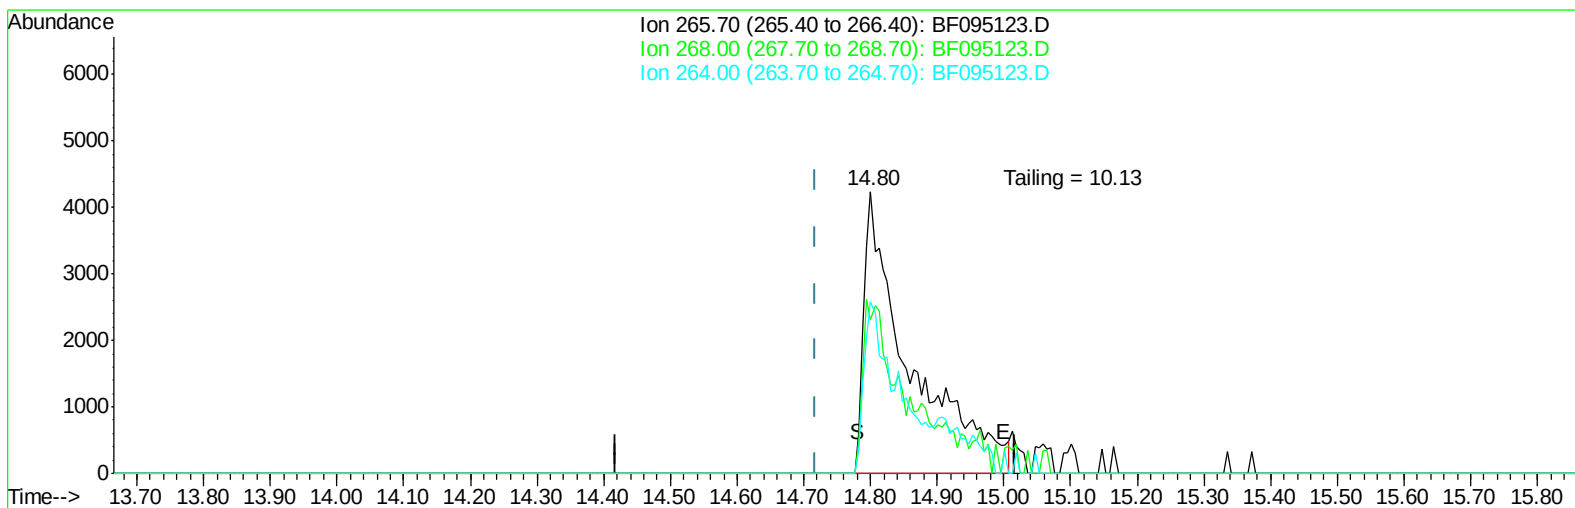

TIC: BF095123.D

(69) Pentachlorophenol (C)

14.801min (+0.082) 0.00ng

response 12032

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	54.61
264.00	64.60	60.75
0.00	0.00	0.00