


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051517\
 Data File : BF095145.D
 Acq On : 16 May 2017 2:44
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

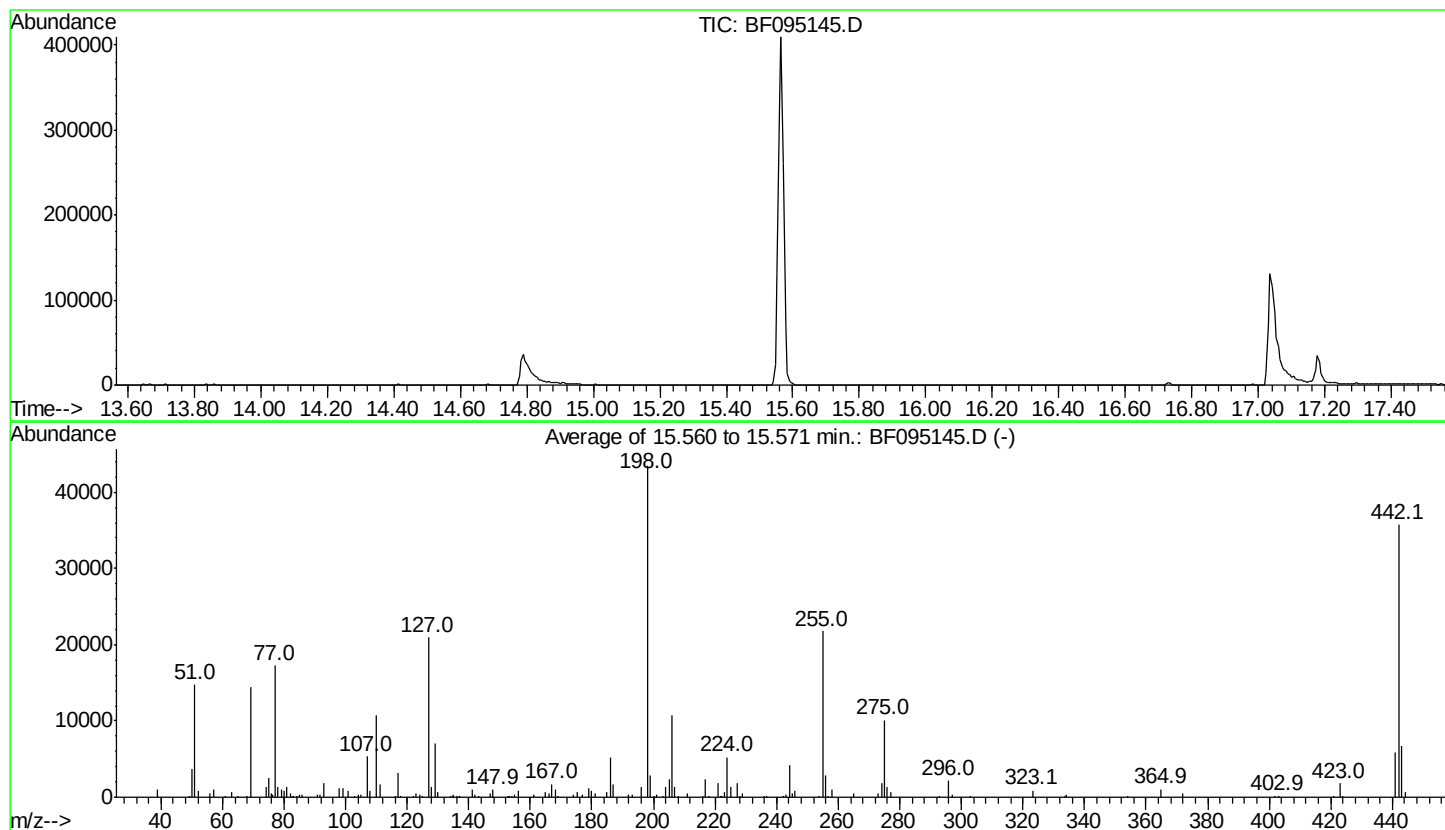

AutoFind: Scans 2316, 2317, 2318; Background Corrected with Scan 2311

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	14692	PASS
68	69	0.00	2	1.0	147	PASS
69	198	0.00	100	33.2	14449	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	20934	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43480	PASS
199	198	5	9	6.6	2881	PASS
275	198	10	60	23.3	10129	PASS
365	198	1	100	2.4	1030	PASS
441	442	0.01	24	16.4	5859	PASS
442	198	50	100	82.2	35746	PASS
443	442	15	24	18.6	6653	PASS