

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051520\
 Data File : BF120318.D
 Acq On : 15 May 2020 13:40
 Operator : MA/SJ
 Sample : PB128905BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB128905BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.228	530	534	562	rBV	6779114	8063334	76.47%	11.531%
2	6.269	707	711	729	rBV	6102716	8174773	77.53%	11.690%
3	6.616	766	770	791	rBV	1394361	1815563	17.22%	2.596%
4	6.769	791	796	819	rBV	5989825	6683761	63.39%	9.558%
5	7.186	861	867	887	rBV	4495224	5473750	51.91%	7.828%
6	7.898	983	988	1016	rBV	2103154	2507615	23.78%	3.586%
7	8.980	1165	1172	1187	rBV	8309365	9461107	89.73%	13.530%
8	9.651	1280	1286	1306	rBV	2887516	3188430	30.24%	4.560%
9	10.445	1415	1421	1441	rBV	5106267	6259209	59.36%	8.951%
10	11.133	1534	1538	1557	rVB	2919644	3081182	29.22%	4.406%
11	12.727	1803	1809	1812	rBV	8915369	10544418	100.00%	15.079%
12	13.768	1981	1986	1994	rBV	2450482	2512854	23.83%	3.593%
13	15.157	2217	2222	2232	rBV	1555865	2043364	19.38%	2.922%
14	16.015	2360	2368	2373	rBV5	44962	119106	1.13%	0.170%


Sum of corrected areas: 69928466

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF051520\
Data File : BF120318.D
Acq On : 15 May 2020 13:40
Operator : MA/SJ
Sample : PB128905BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128905BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

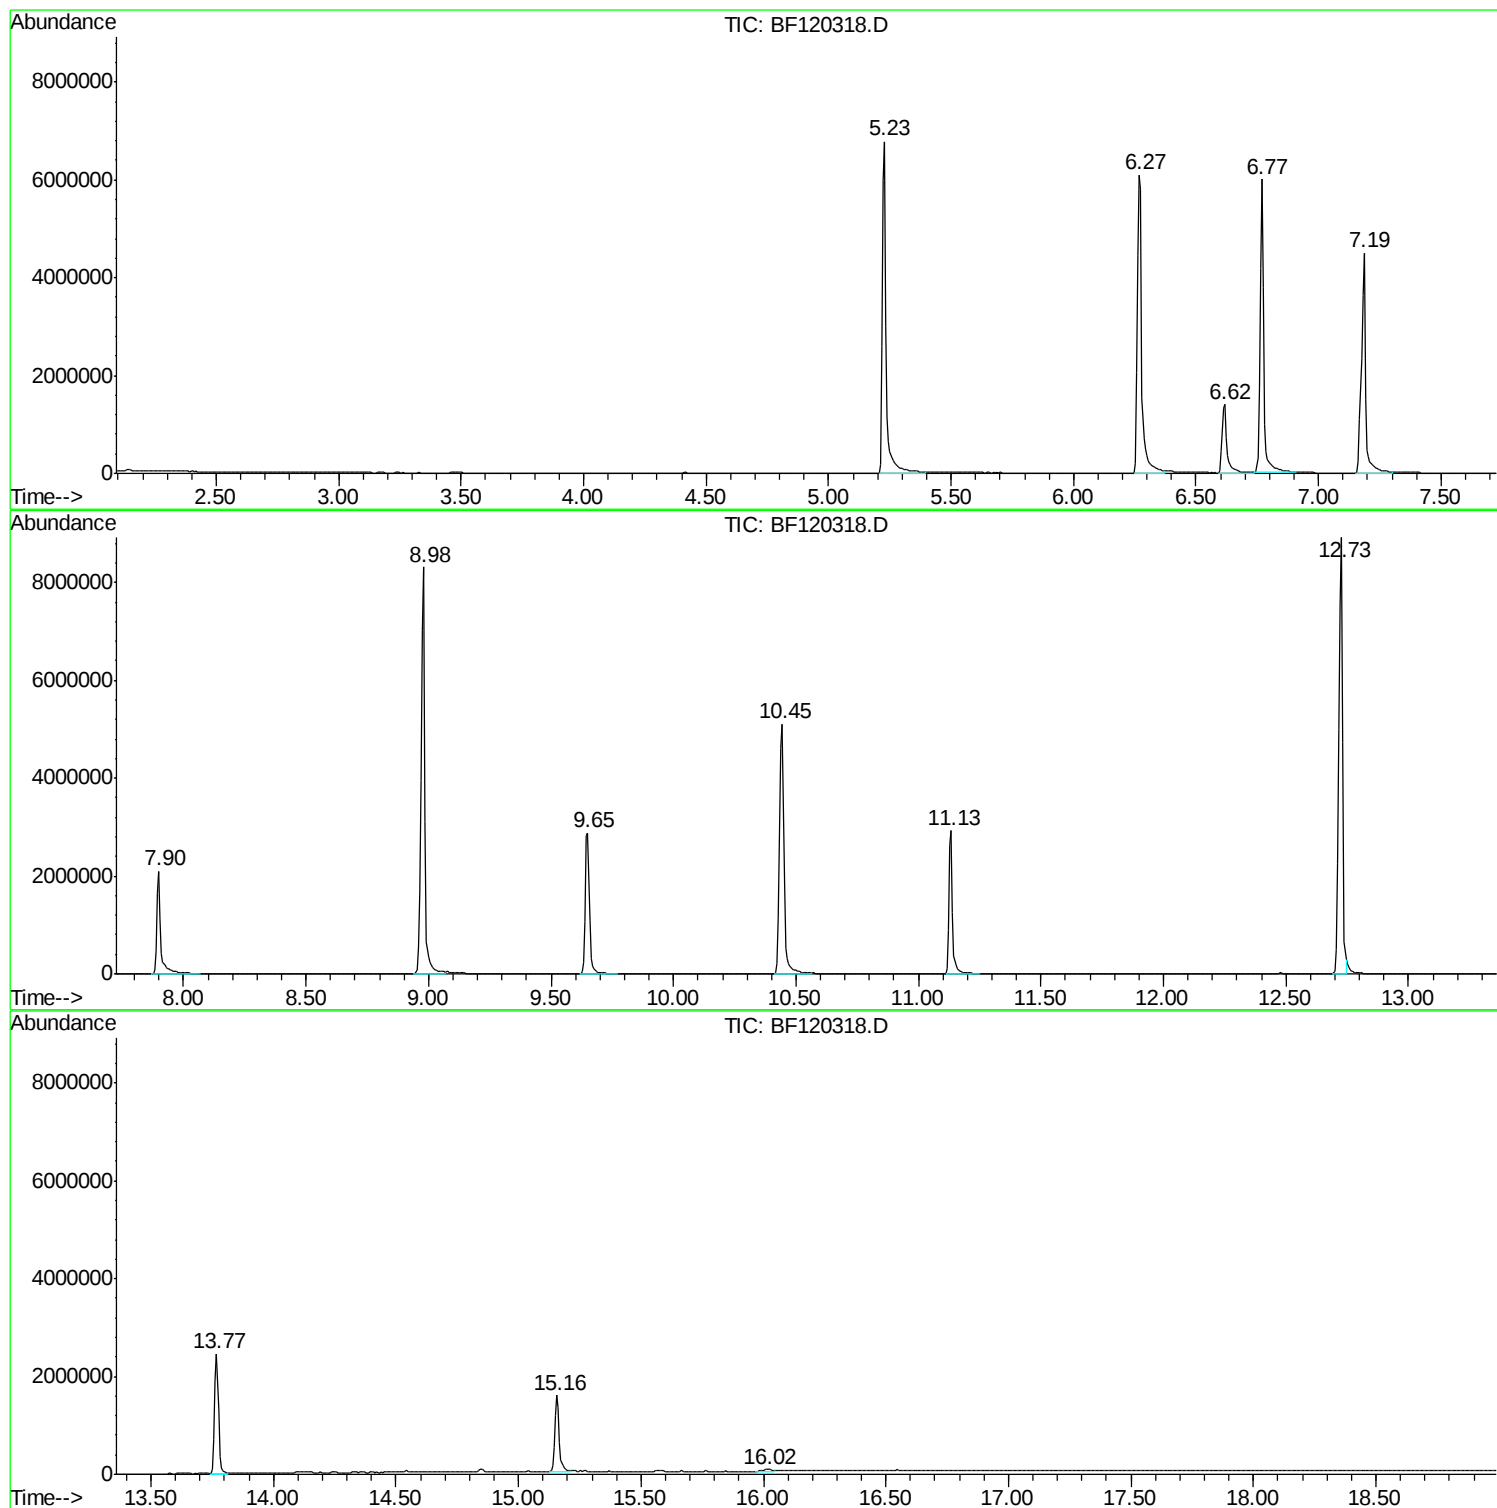

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051520\
Data File : BF120318.D
Acq On : 15 May 2020 13:40
Operator : MA/SJ
Sample : PB128905BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128905BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051520\
Data File : BF120318.D
Acq On : 15 May 2020 13:40
Operator : MA/SJ
Sample : PB128905BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB128905BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc