


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051520\
 Data File : BF120313.D
 Acq On : 15 May 2020 11:19
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 15 12:31:31 2020

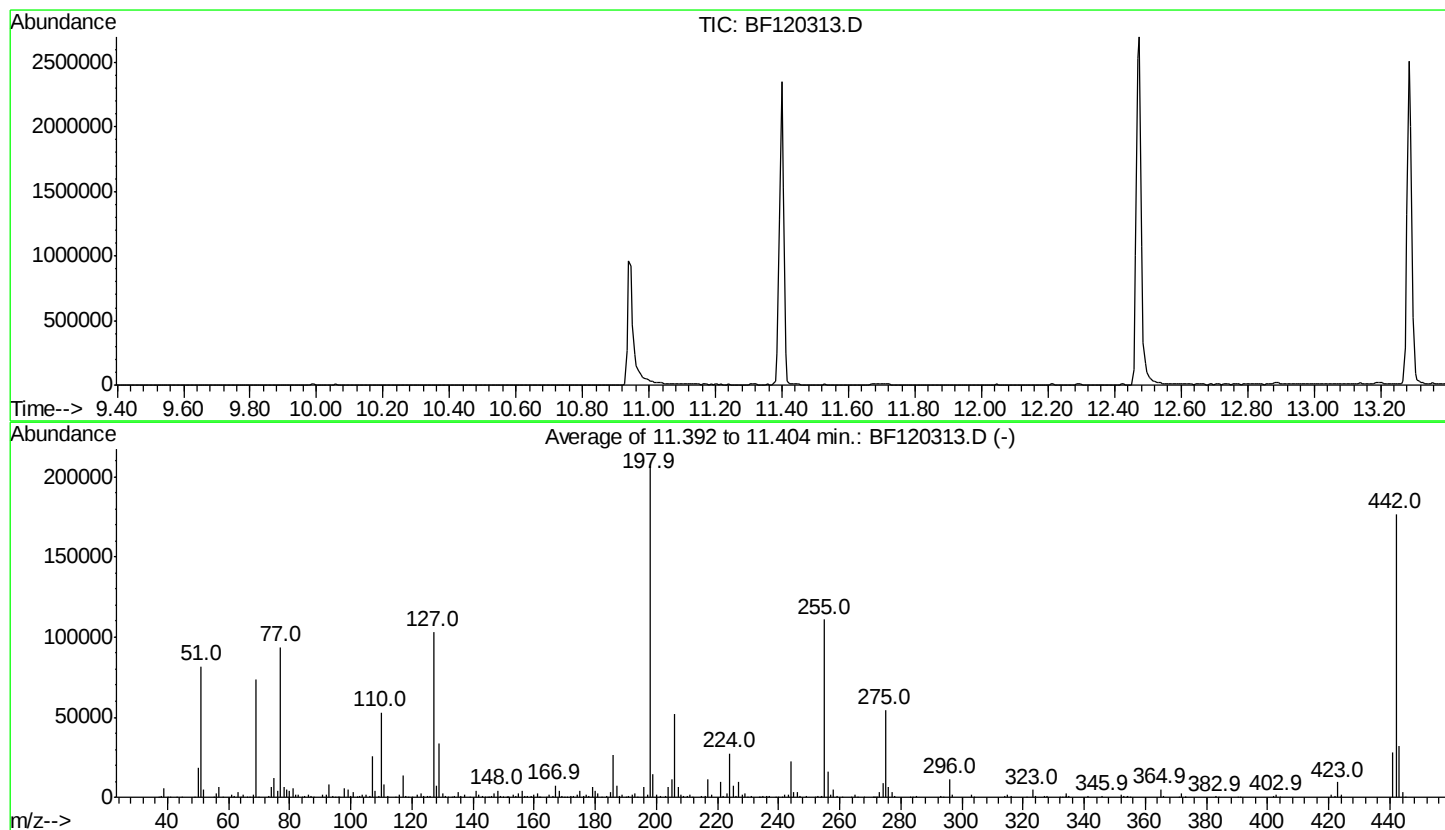

AutoFind: Scans 1582, 1583, 1584; Background Corrected with Scan 1576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	81992	PASS
68	69	0.00	2	1.7	1260	PASS
69	198	0.00	100	35.6	73666	PASS
70	69	0.00	2	0.5	391	PASS
127	198	10	80	49.9	103344	PASS
197	198	0.00	2	0.6	1335	PASS
198	198	100	100	100.0	207168	PASS
199	198	5	9	6.9	14398	PASS
275	198	10	60	26.3	54469	PASS
365	198	1	100	2.4	5040	PASS
441	198	0.01	100	13.7	28295	PASS
442	198	50	100	85.4	176853	PASS
443	442	15	24	18.1	31985	PASS