
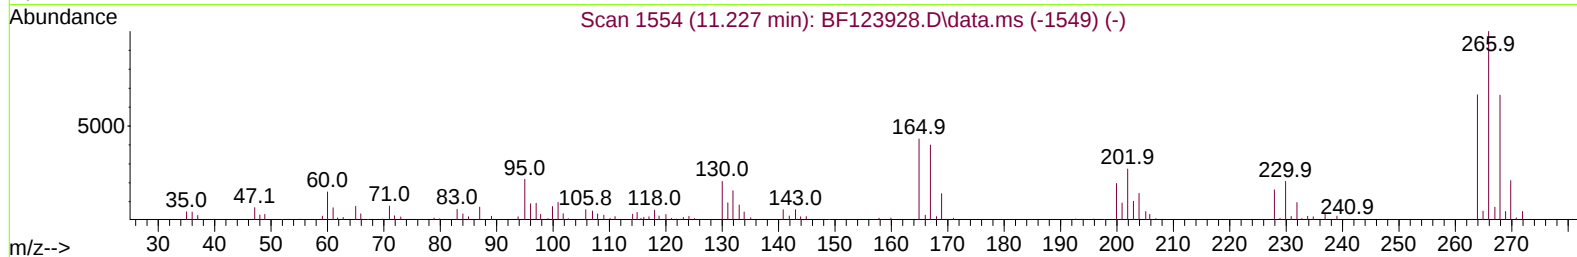
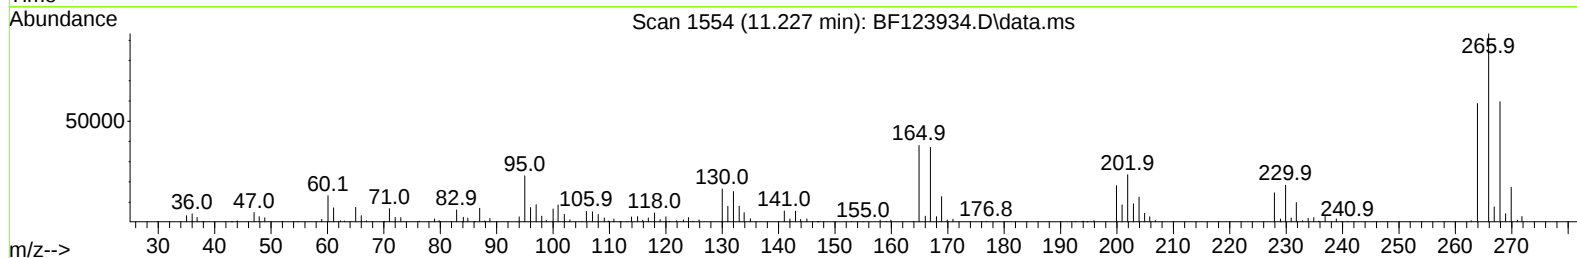


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051521\
Data File : BF123934.D
Acq On : 15 May 2021 8:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 05:51:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

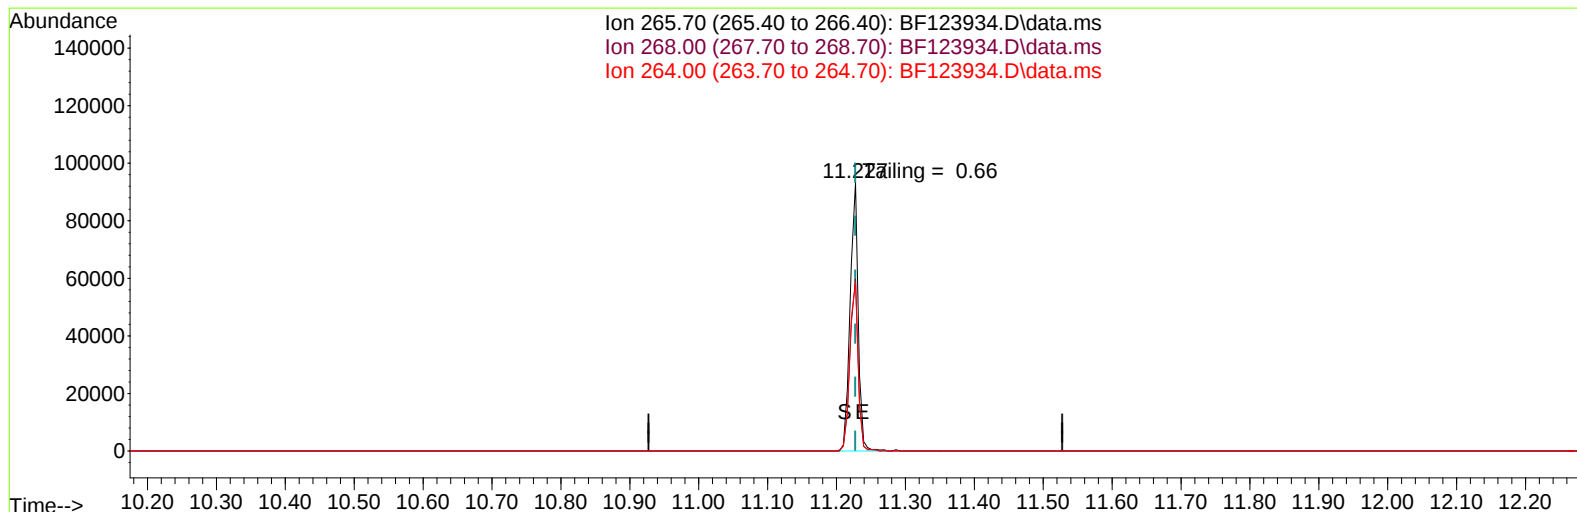

TIC: BF123934.D\data.ms

(70) Pentachlorophenol (C)




11.227min (+ 0.000) 51477.11 ng

response 75669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.03
264.00	65.70	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051521\
 Data File : BF123934.D
 Acq On : 15 May 2021 8:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 05:51:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

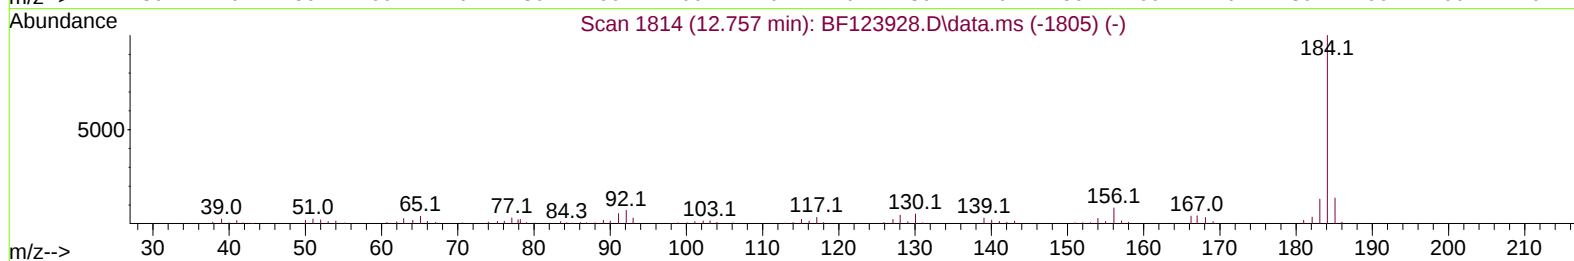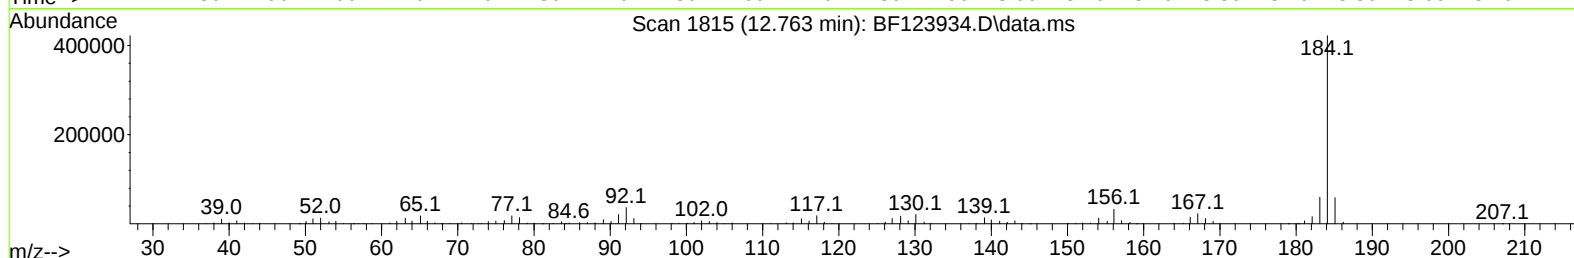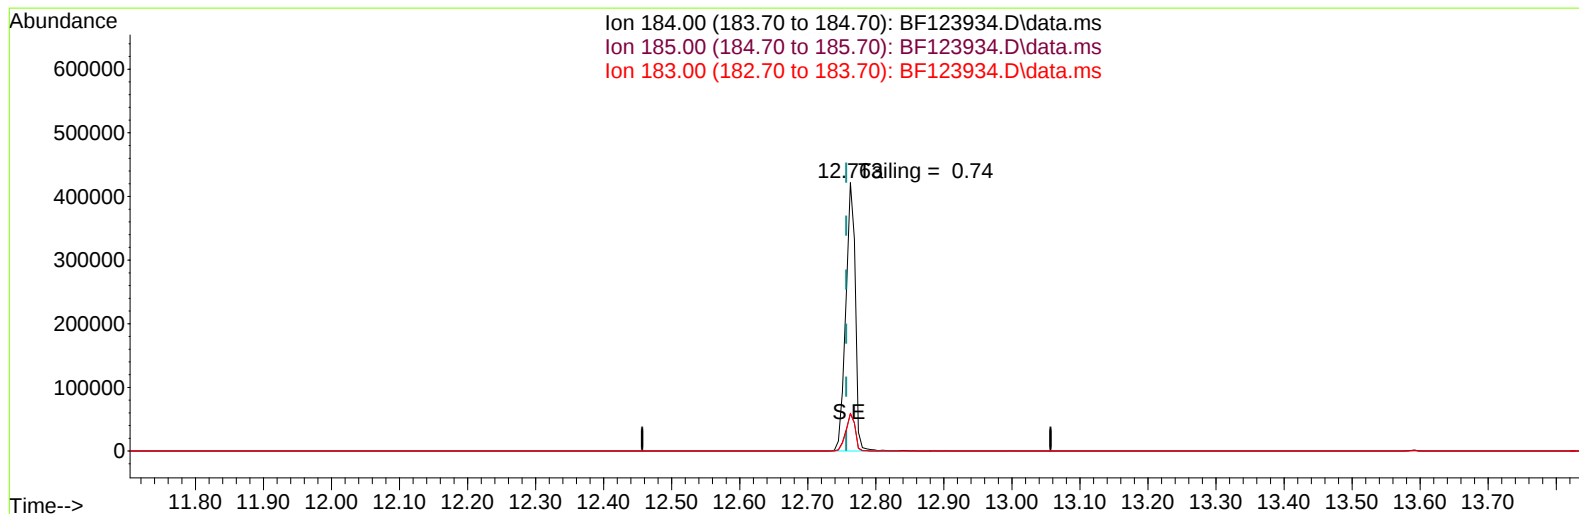

TIC: BF123934.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 409752

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.92
183.00	9.80	14.14#
0.00	0.00	0.00