
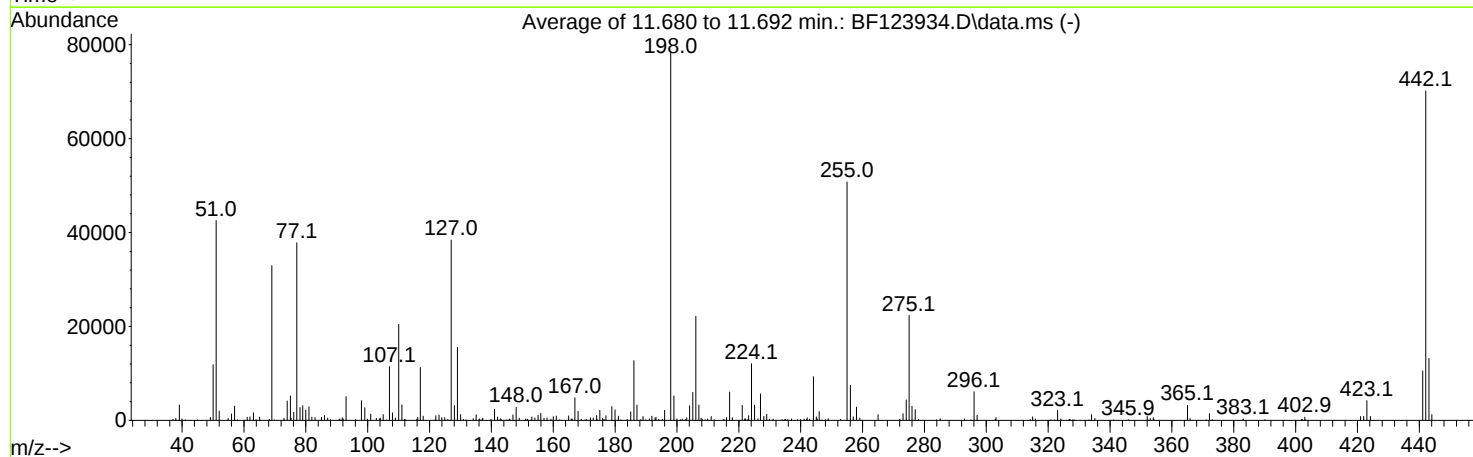


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051521\
 Data File : BF123934.D
 Acq On : 15 May 2021 8:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 14 19:05:57 2021

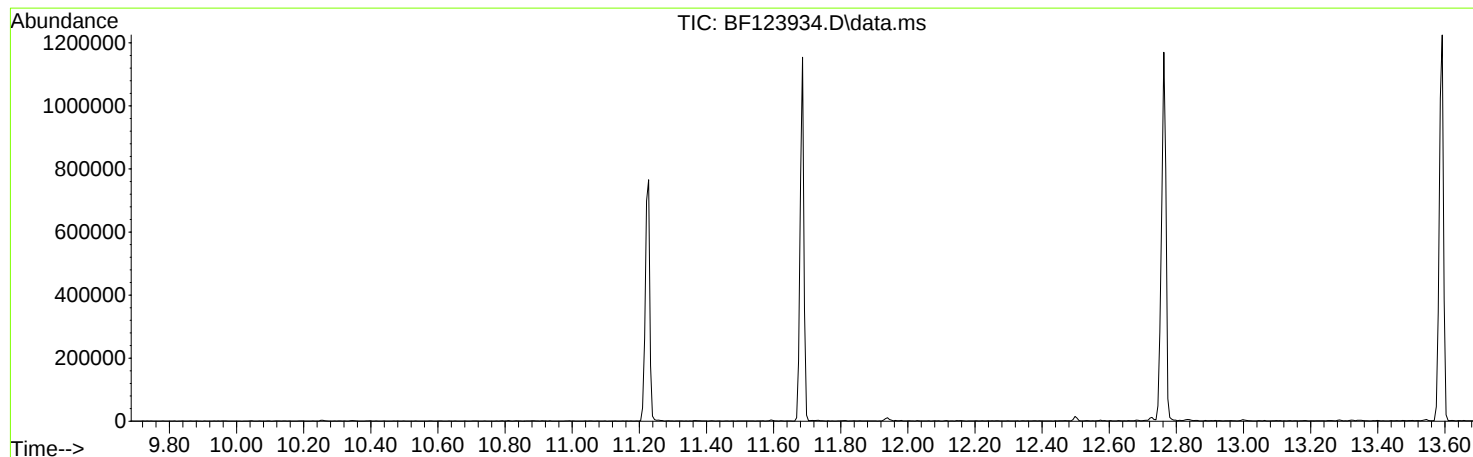

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.3	42554	PASS
68	69	0.00	2	0.6	214	PASS
69	198	0.00	100	42.1	32969	PASS
70	69	0.00	2	0.3	104	PASS
127	198	10	80	49.0	38415	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78347	PASS
199	198	5	9	6.7	5217	PASS
275	198	10	60	28.5	22347	PASS
365	198	1	100	4.1	3210	PASS
441	198	0.01	100	13.5	10548	PASS
442	442	50	100	100.0	70179	PASS
443	442	15	24	18.8	13188	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/15/2021	BNA_F	<u>BF123934.D</u>
Compound Name	Response	Retention Time
DDT	191311	13.592
DDD	1167	13.286
DDE	261	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1428	192739	0.74

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051521\
 Data File : BF123934.D
 Acq On : 15 May 2021 8:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 16 05:51:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 19:05:57 2021
 Response via : Initial Calibration

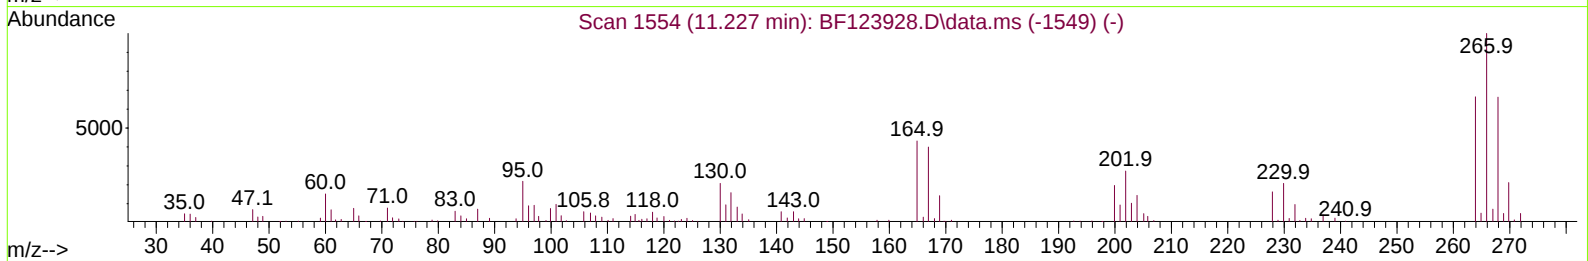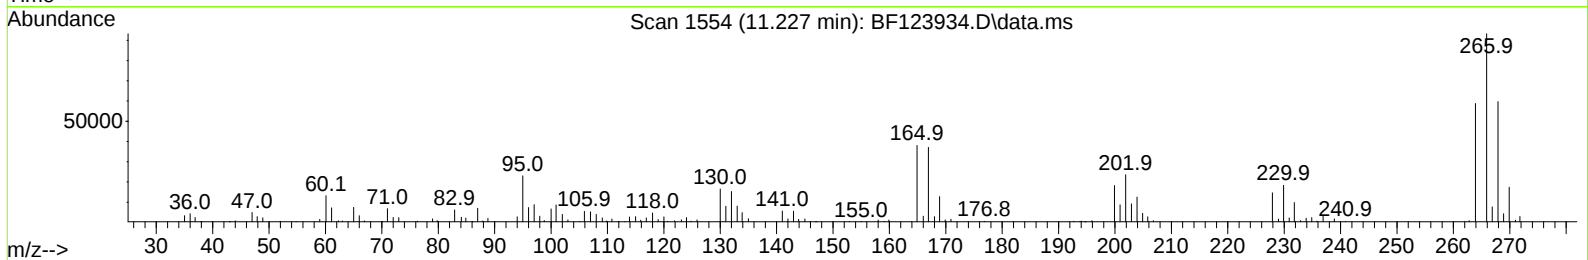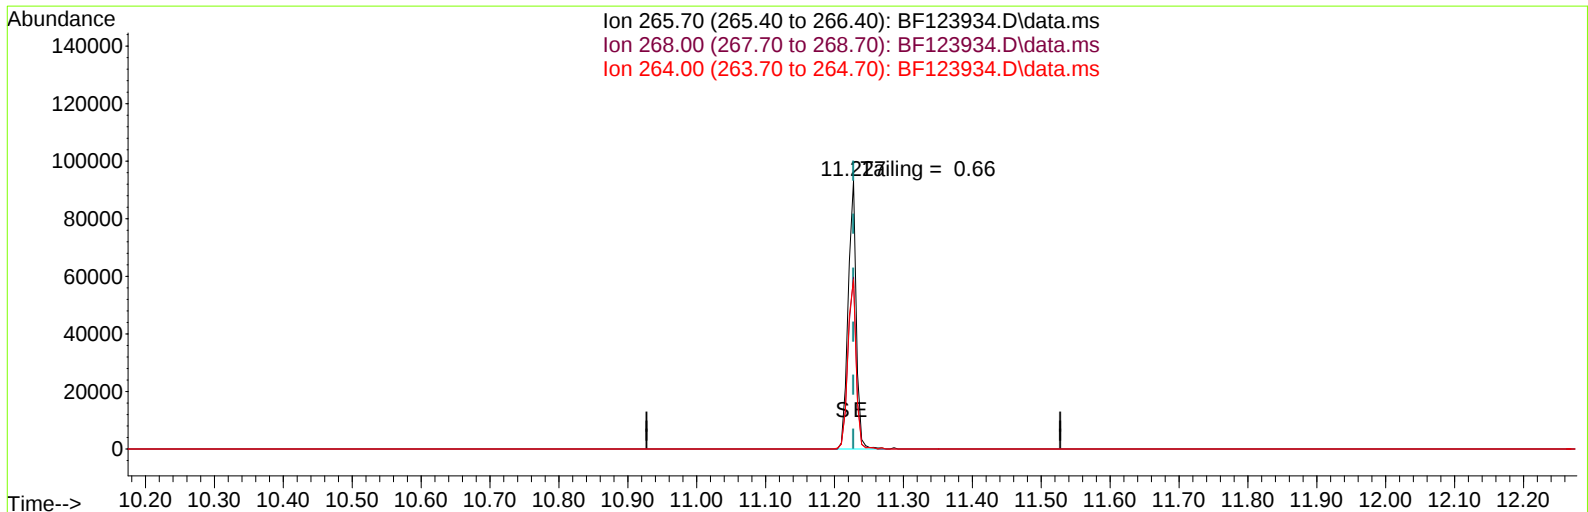

TIC: BF123934.D\data.ms

(70) Pentachlorophenol (C)

11.227min (+ 0.000) 51477.11 ng




response 75669

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.03
264.00	65.70	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051521\
Data File : BF123934.D
Acq On : 15 May 2021 8:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 16 05:51:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 19:05:57 2021
Response via : Initial Calibration

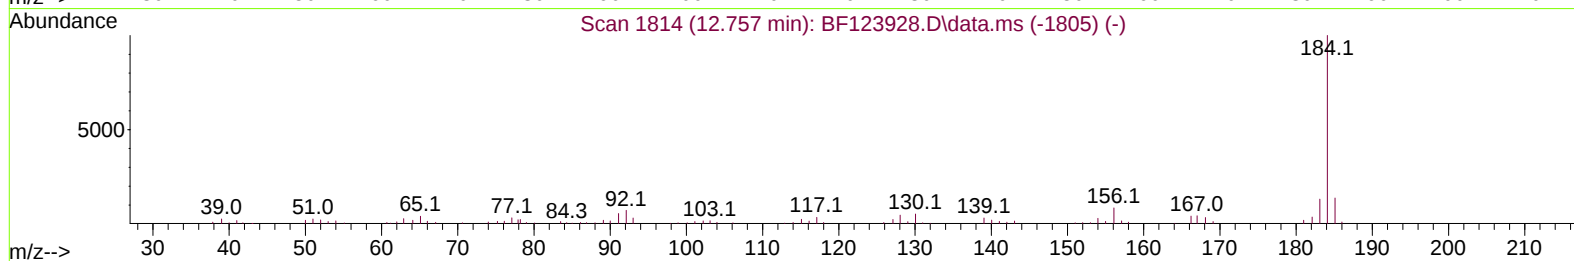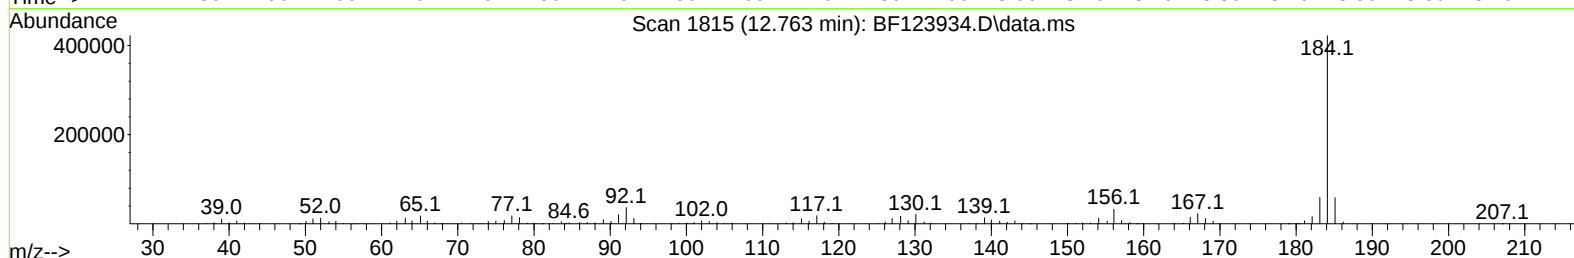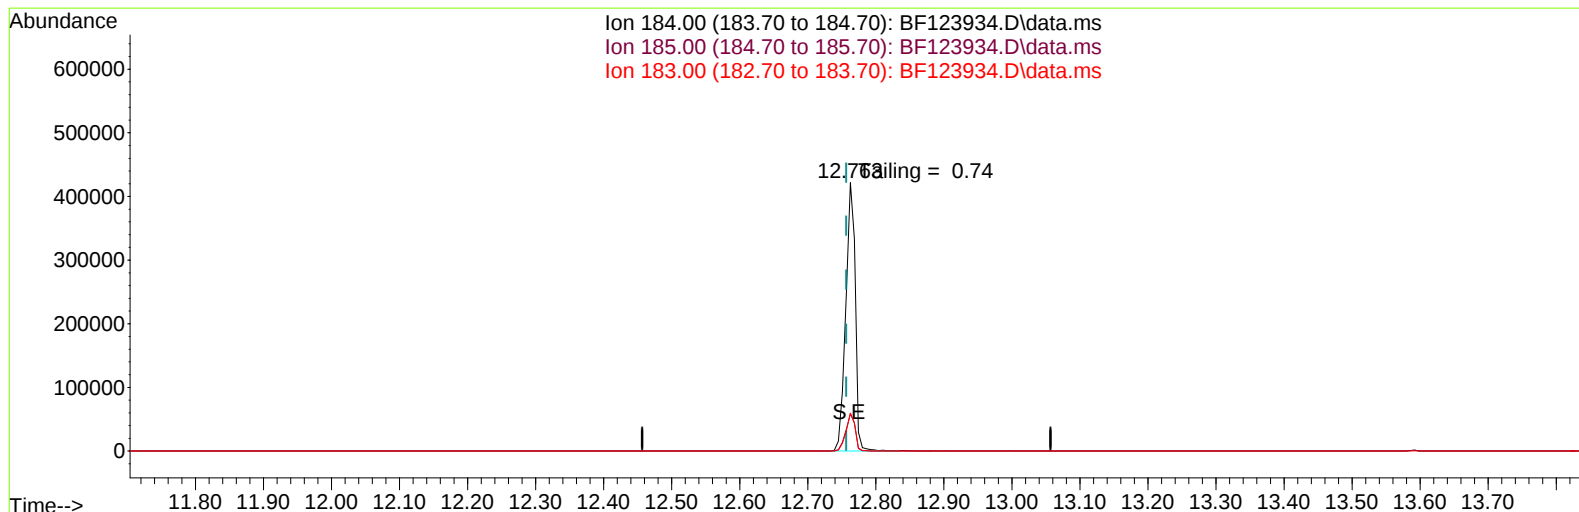

TIC: BF123934.D\data.ms

(77) Benzidine

12.763min (+ 0.006) 0.00 ng

response 409752

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.92
183.00	9.80	14.14#
0.00	0.00	0.00