
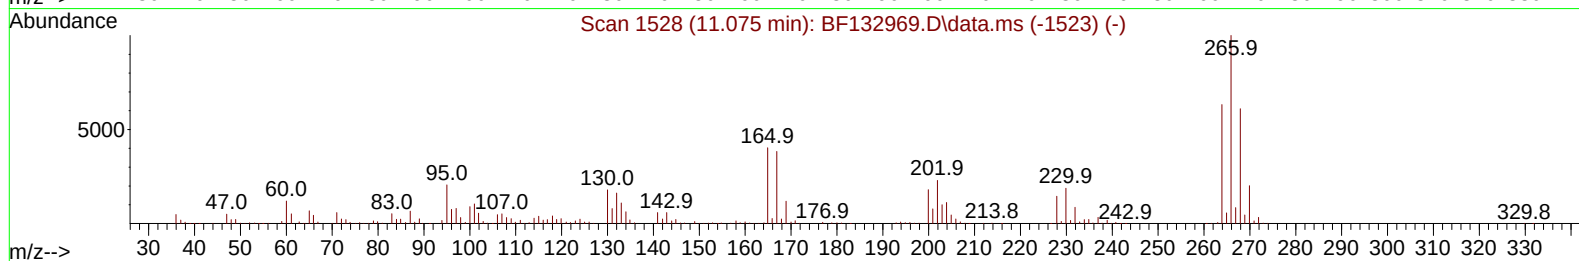
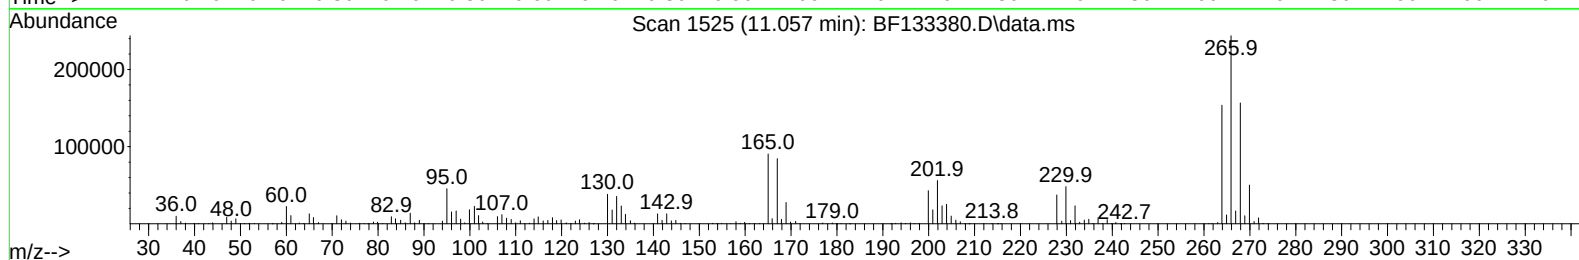


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051523\
Data File : BF133380.D
Acq On : 15 May 2023 10:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 13:48:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 16:40:17 2023
Response via : Initial Calibration

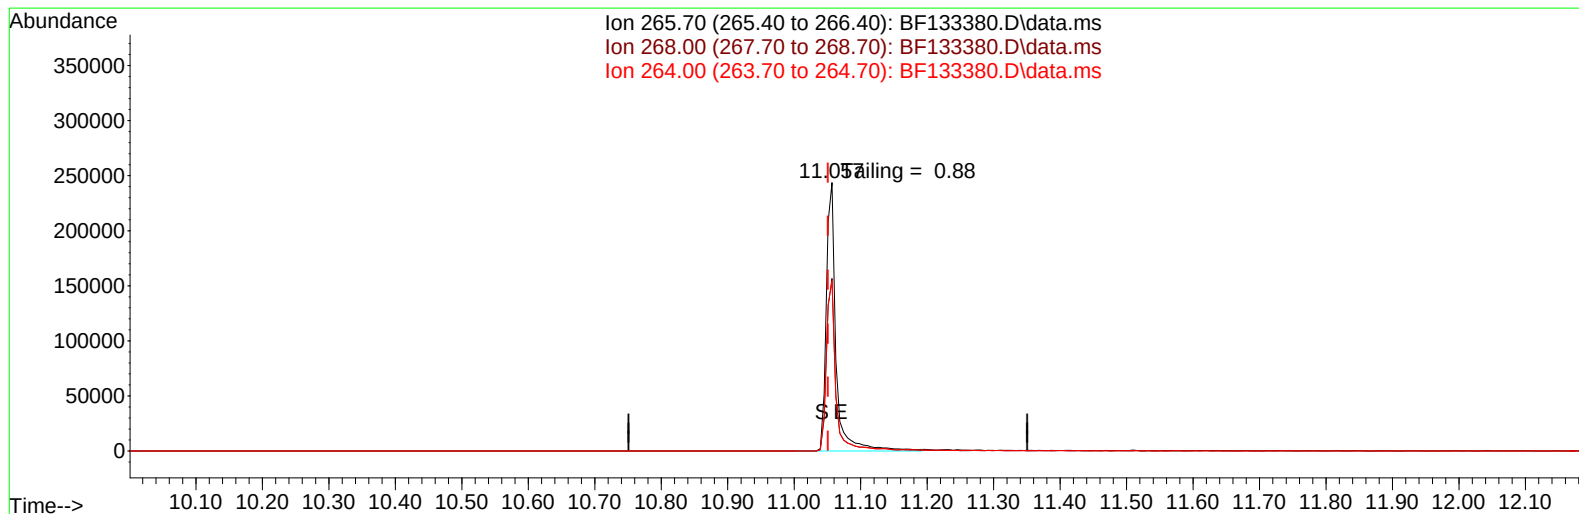

TIC: BF133380.D\data.ms

(70) Pentachlorophenol (C)




11.057min (+ 0.006) 25438.17 ng

response 249258

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.26
264.00	63.30	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051523\
 Data File : BF133380.D
 Acq On : 15 May 2023 10:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 13:48:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 11 16:40:17 2023
 Response via : Initial Calibration

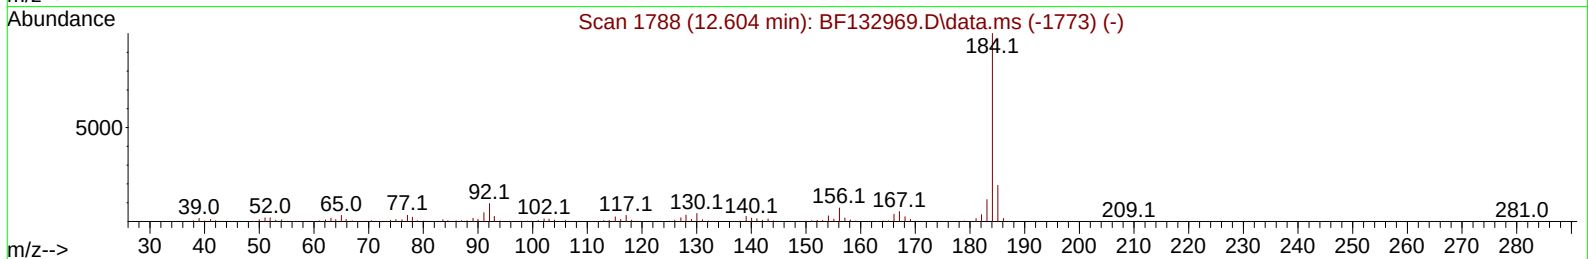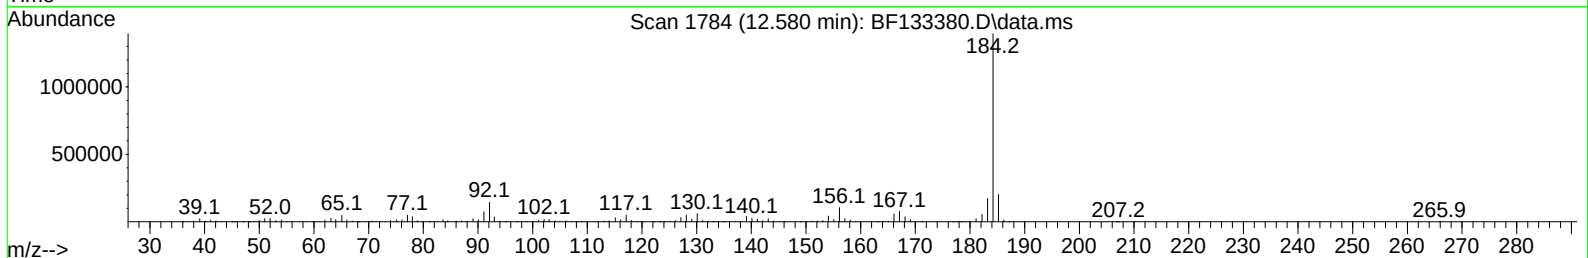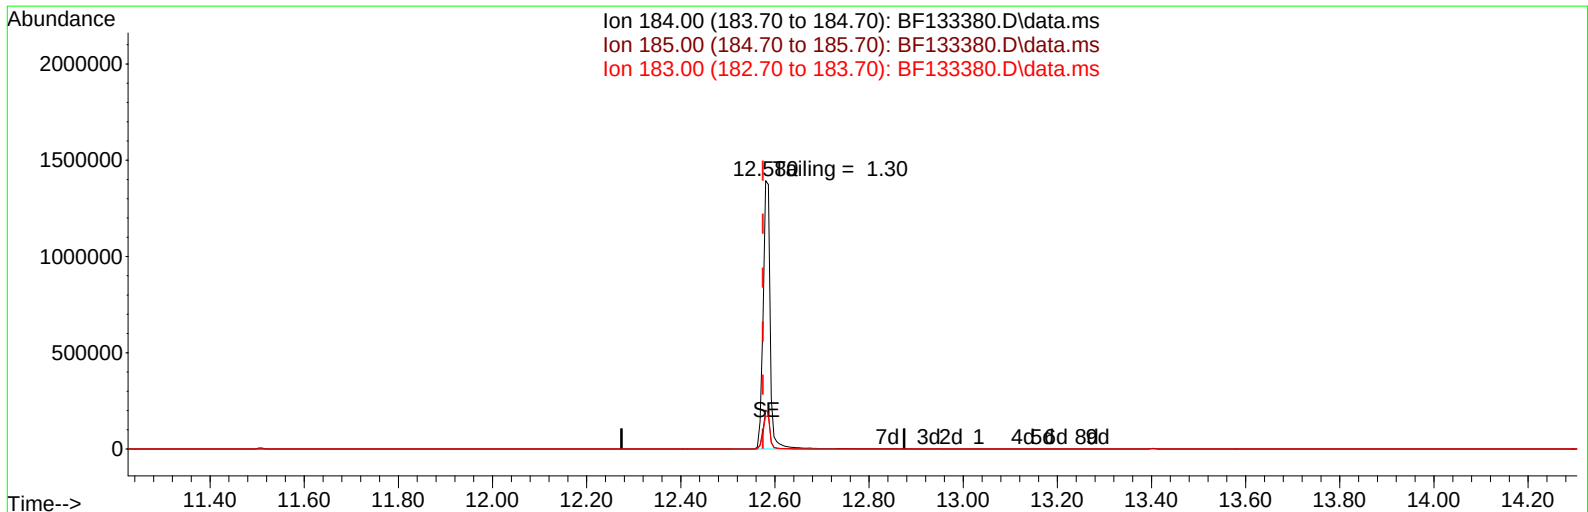

TIC: BF133380.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 1606072.89 ng m

response 1466615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.52#
183.00	11.70	12.33
0.00	0.00	0.00