
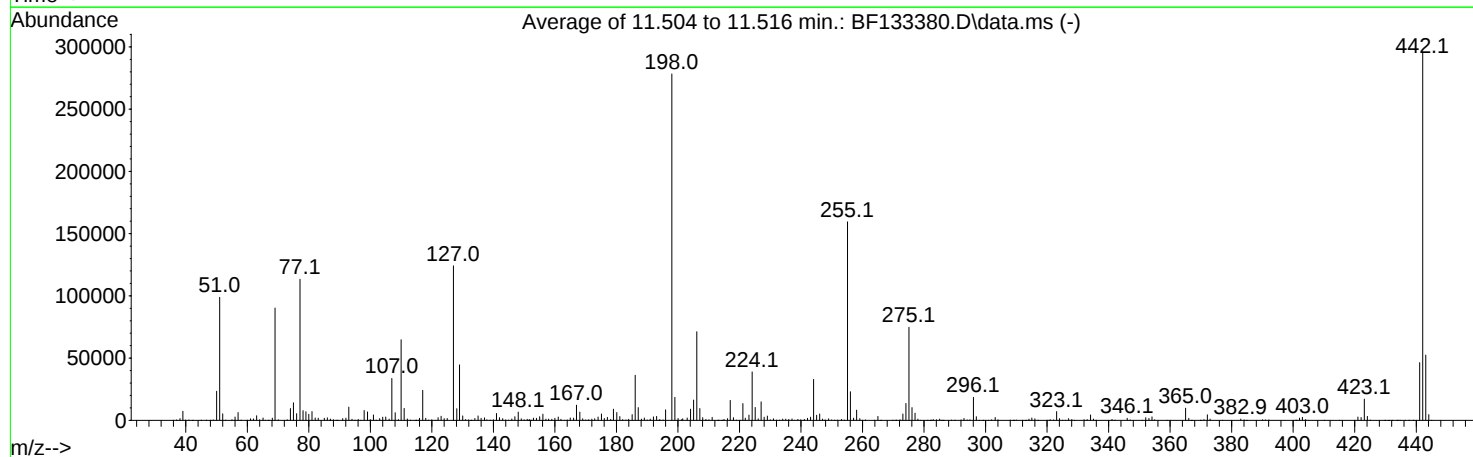


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051523\
 Data File : BF133380.D
 Acq On : 15 May 2023 10:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 16:40:17 2023

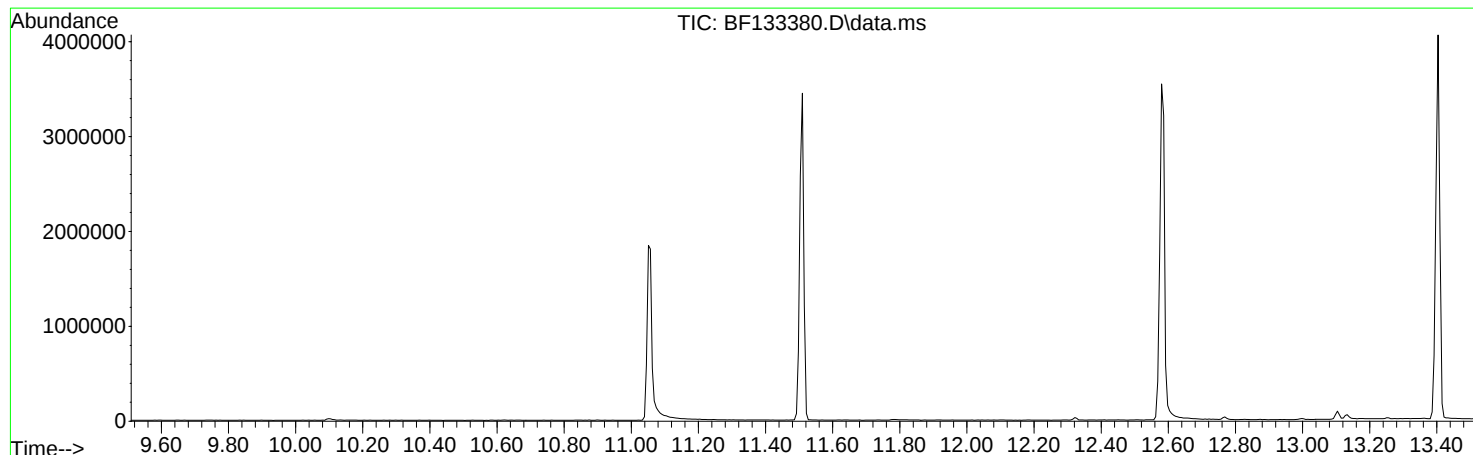

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	98867	PASS
68	69	0.00	2	2.0	1792	PASS
69	198	0.00	100	32.4	90203	PASS
70	69	0.00	2	0.6	549	PASS
127	198	10	80	44.6	124136	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	278291	PASS
199	198	5	9	6.6	18477	PASS
275	198	10	60	26.9	74832	PASS
365	198	1	100	3.5	9786	PASS
441	198	0.01	100	16.7	46352	PASS
442	442	50	100	100.0	295509	PASS
443	442	15	24	17.8	52464	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
5/15/2023	BNA_F	<u>BF133380.D</u>
Compound Name	Response	Retention Time
DDT	661858	13.404
DDD	20448	13.104
DDE	3310	12.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23758	685616	3.47

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051523\
 Data File : BF133380.D
 Acq On : 15 May 2023 10:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 15 13:48:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 11 16:40:17 2023
 Response via : Initial Calibration

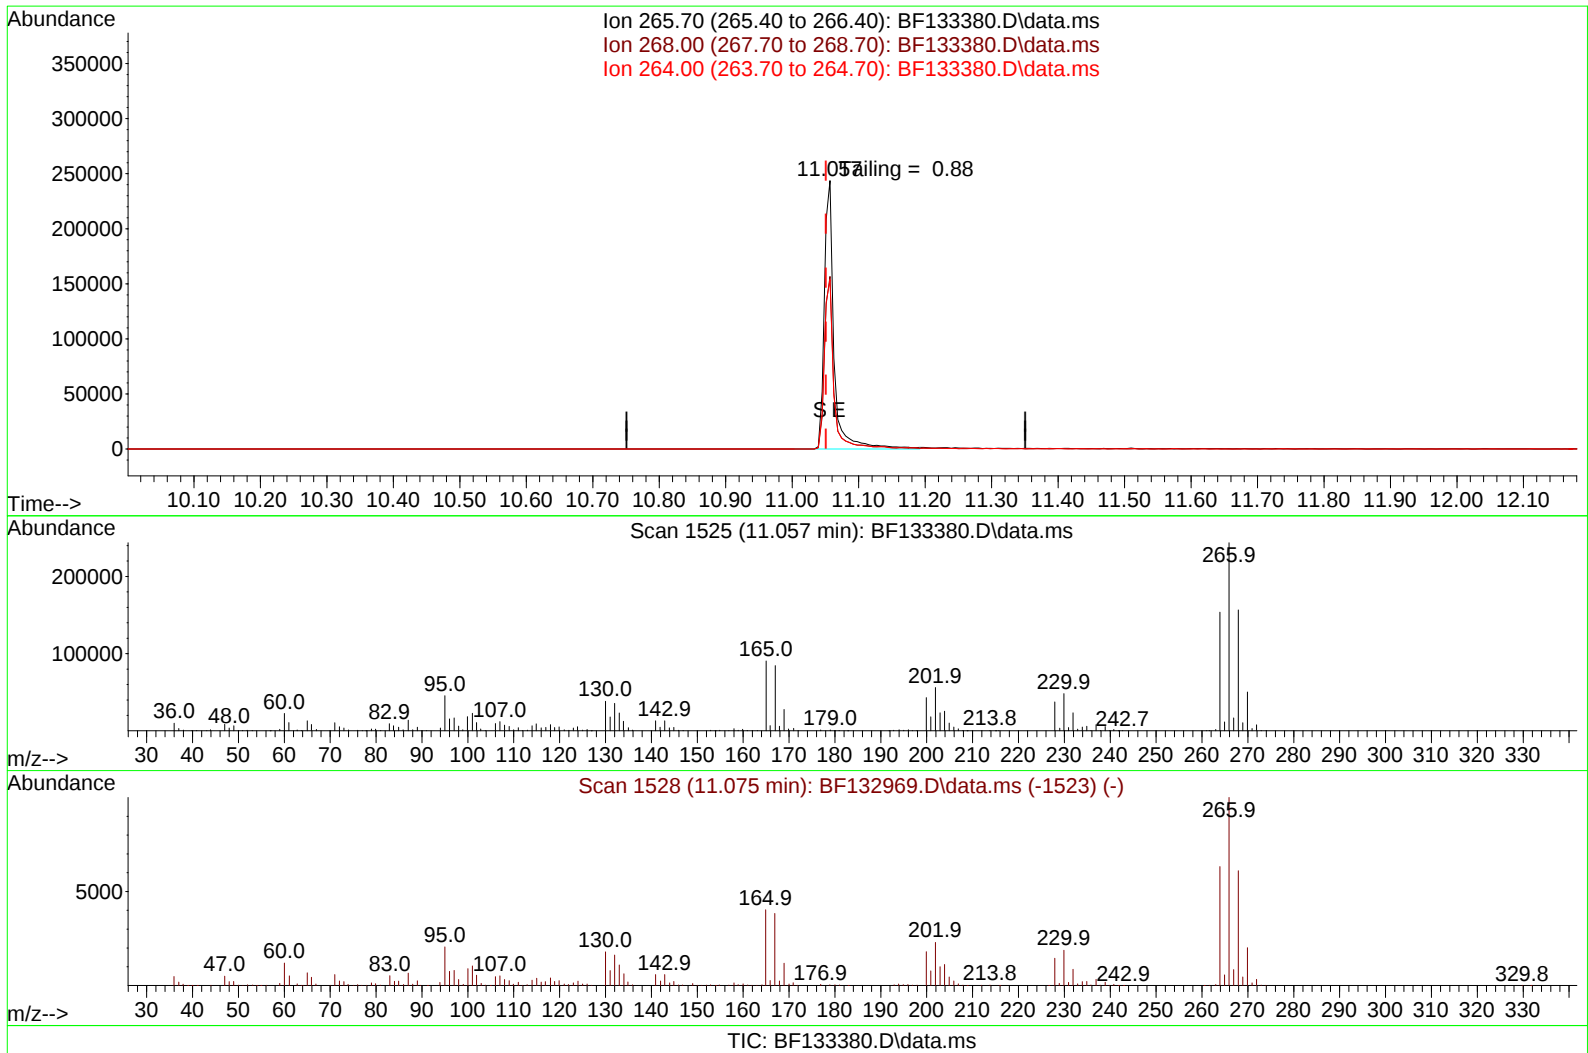

(70) Pentachlorophenol (C)

11.057min (+ 0.006) 25438.17 ng


response 249258

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.26
264.00	63.30	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051523\
 Data File : BF133380.D
 Acq On : 15 May 2023 10:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 15 13:48:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 11 16:40:17 2023
 Response via : Initial Calibration

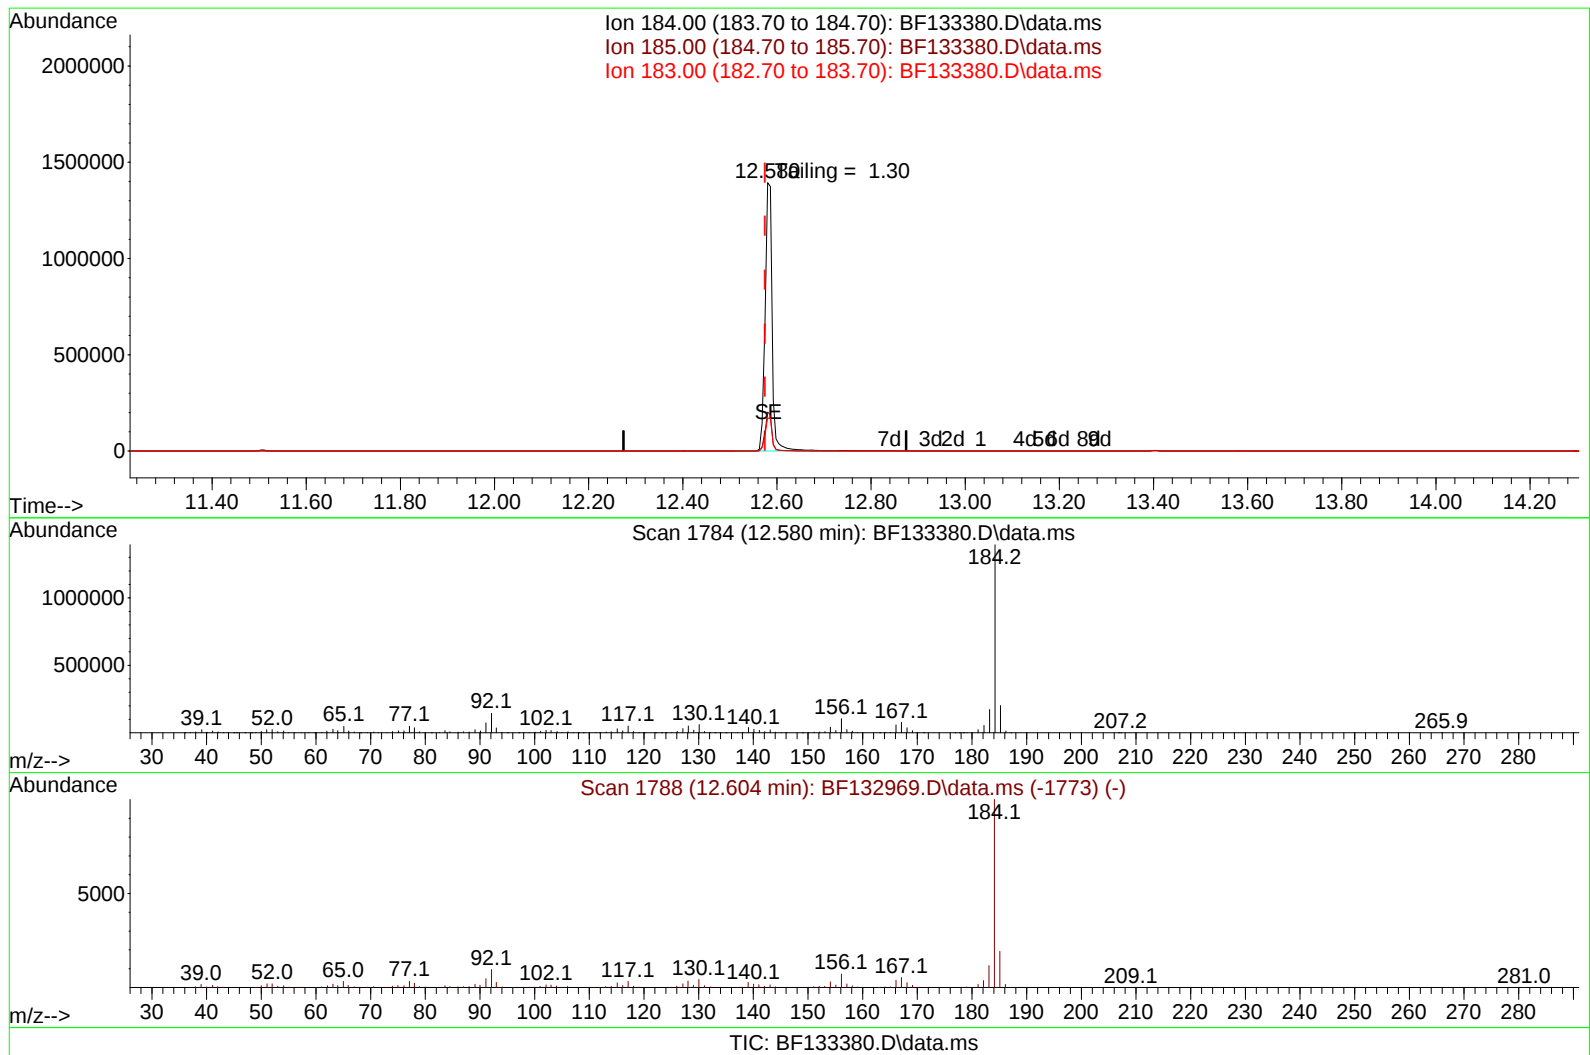

(77) Benzidine

12.580min (+ 0.006) 1606072.89 ng m

response 1466615

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.52#
183.00	11.70	12.33
0.00	0.00	0.00