
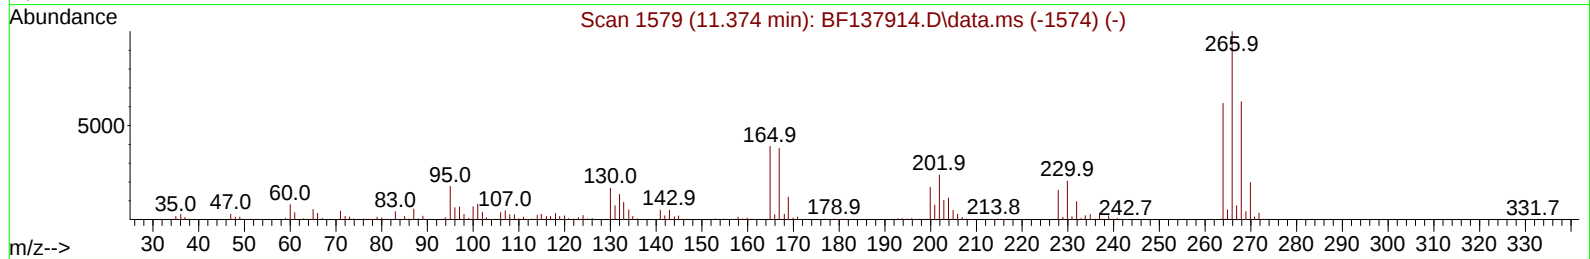
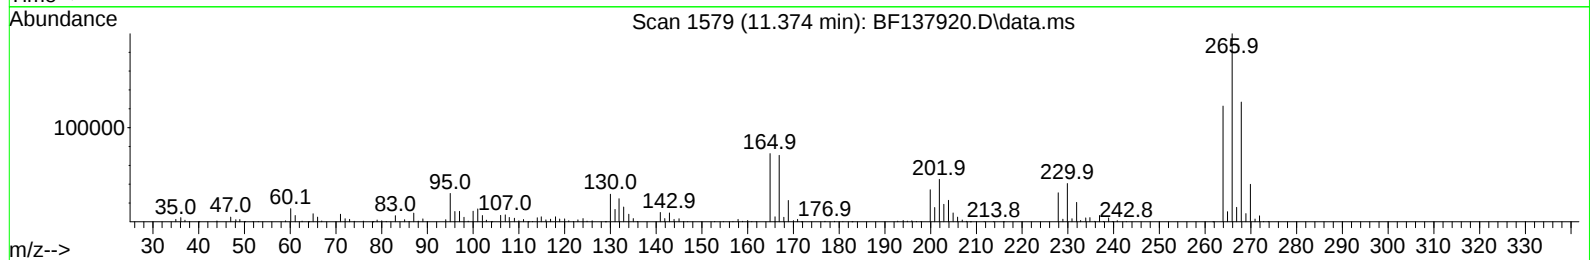


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051524\
Data File : BF137920.D
Acq On : 15 May 2024 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 11:34:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

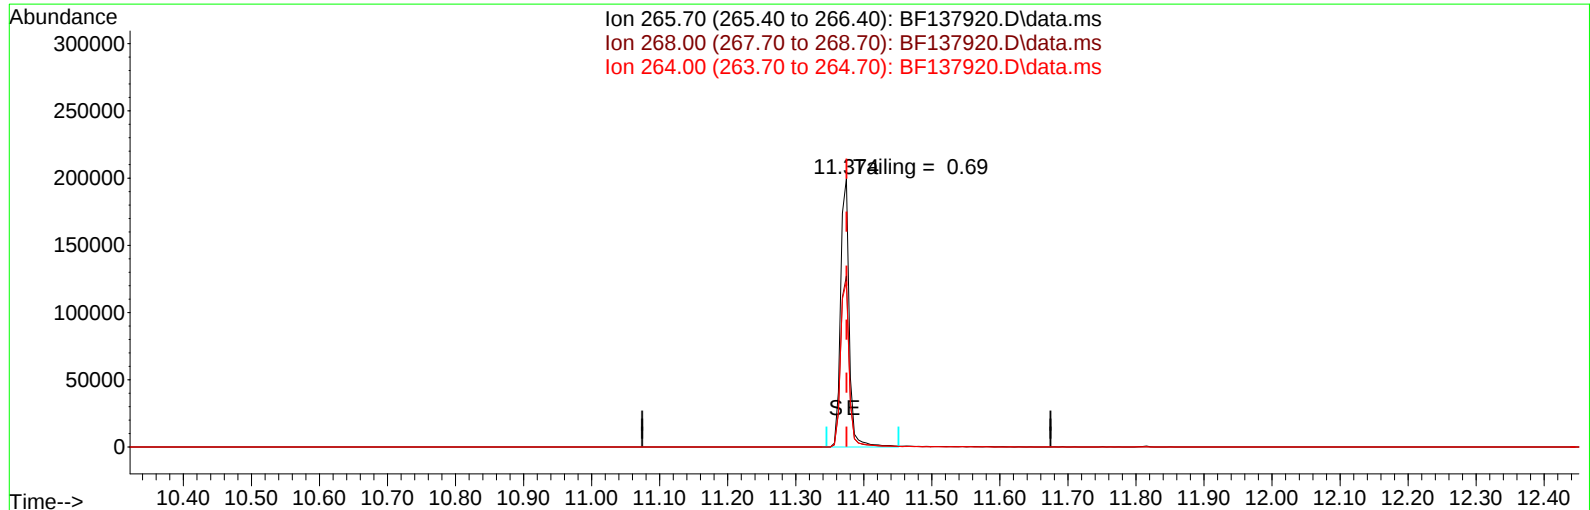

TIC: BF137920.D\data.ms

(70) Pentachlorophenol (C)




11.374min (+ 0.000) 24326.40 ng

response 176478

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.67
264.00	61.80	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051524\
Data File : BF137920.D
Acq On : 15 May 2024 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 15 11:34:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

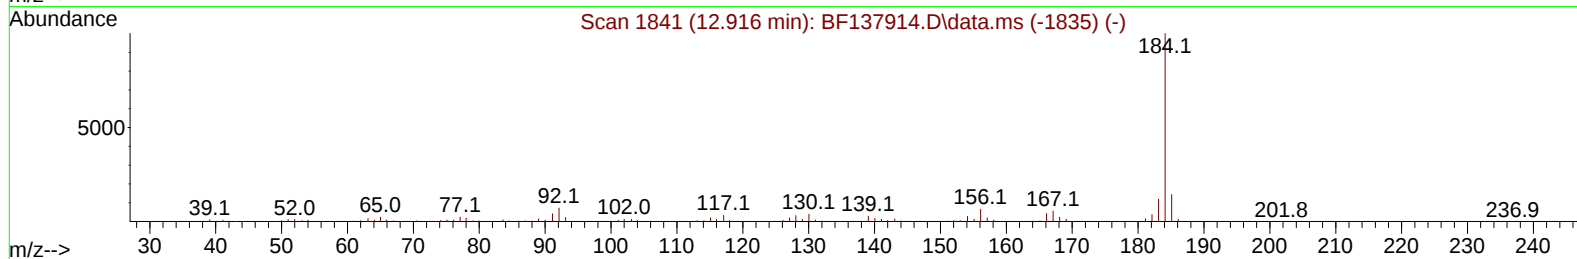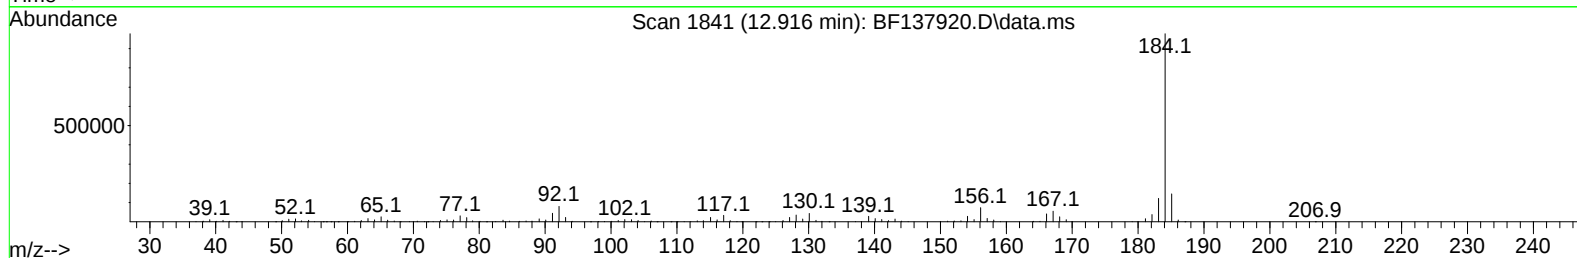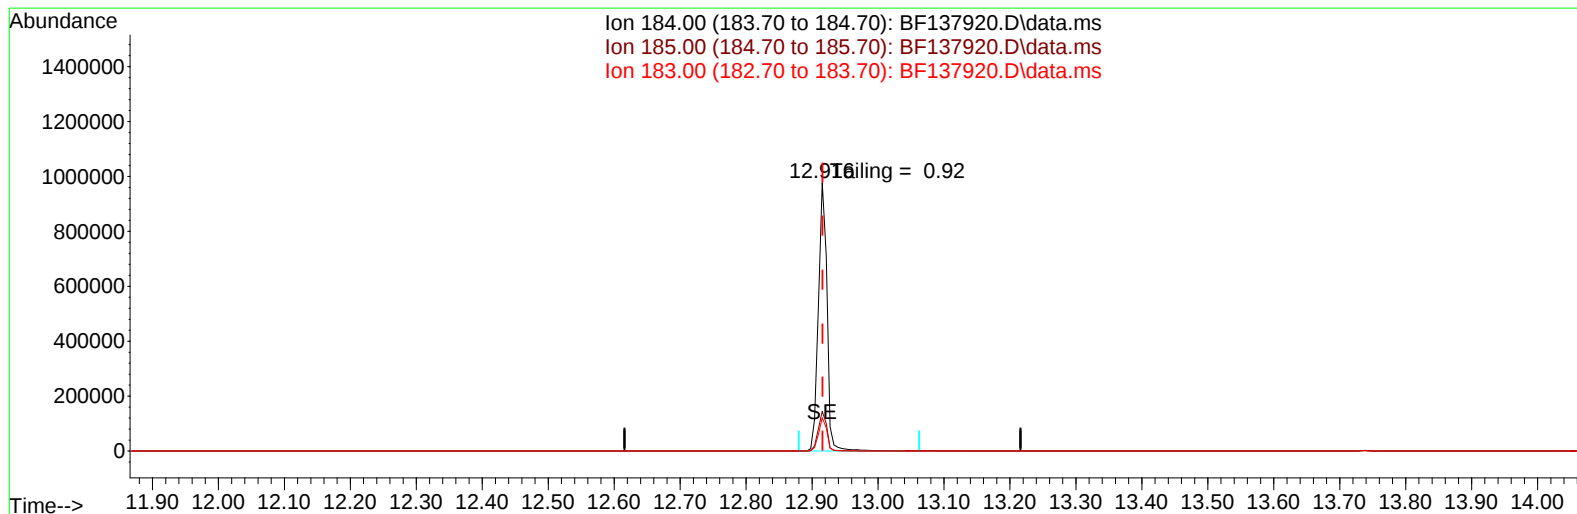

TIC: BF137920.D\data.ms

(77) Benzidine

12.916min (-0.000) 0.00 ng

response 889390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.80
183.00	11.90	12.43
0.00	0.00	0.00