


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051524\
Data File : BF137920.D
Acq On : 15 May 2024 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

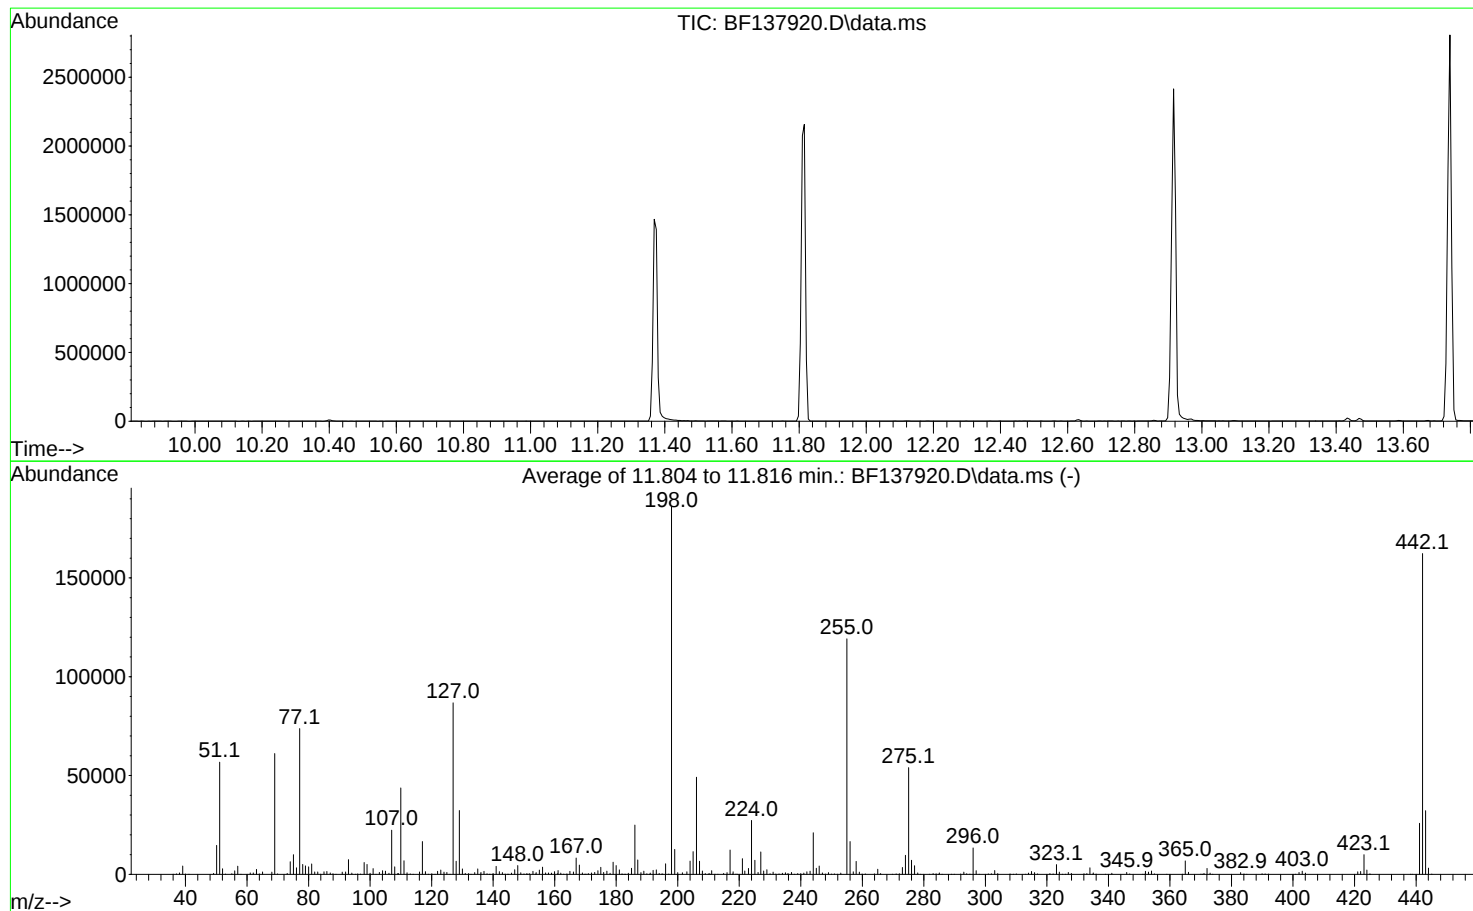

AutoFind: Scans 1652, 1653, 1654; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	56755	PASS
68	69	0.00	2	1.8	1100	PASS
69	198	0.00	100	32.8	61125	PASS
70	69	0.00	2	0.4	244	PASS
127	198	10	80	46.6	86827	PASS
197	198	0.00	2	0.1	190	PASS
198	198	100	100	100.0	186139	PASS
199	198	5	9	6.8	12676	PASS
275	198	10	60	29.0	54007	PASS
365	198	1	100	3.7	6836	PASS
441	198	0.01	100	13.9	25840	PASS
442	442	50	100	100.0	162315	PASS
443	442	15	24	19.8	32192	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/15/2024	BNA_F	<u>BF137920.D</u>
Compound Name	Response	Retention Time
DDT	456636	13.739
DDD	7489	13.433
DDE	590	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8079	464715	1.74

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051524\
Data File : BF137920.D
Acq On : 15 May 2024 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 15 11:34:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

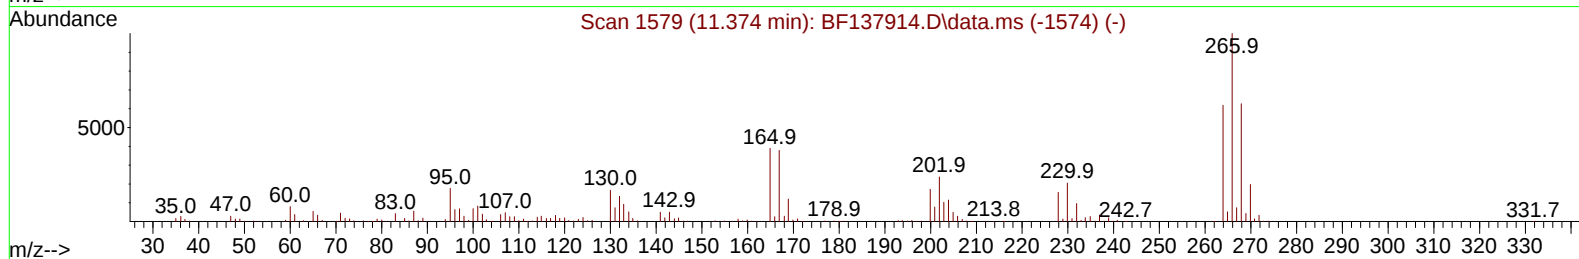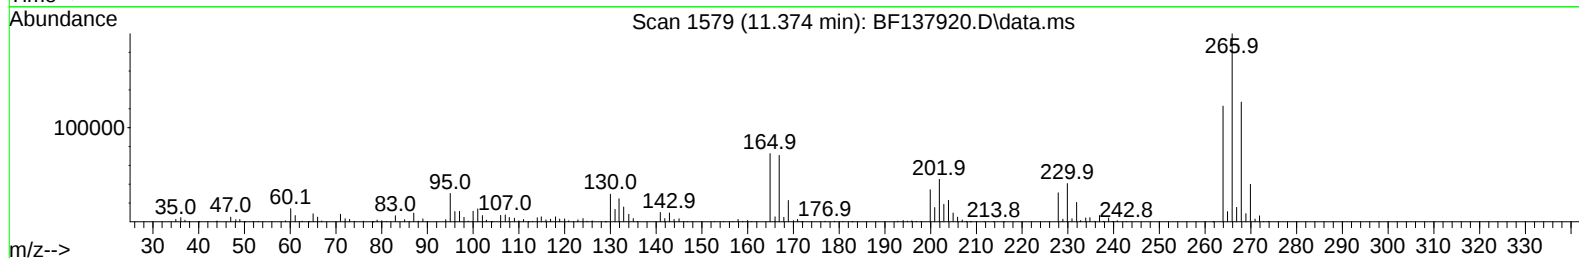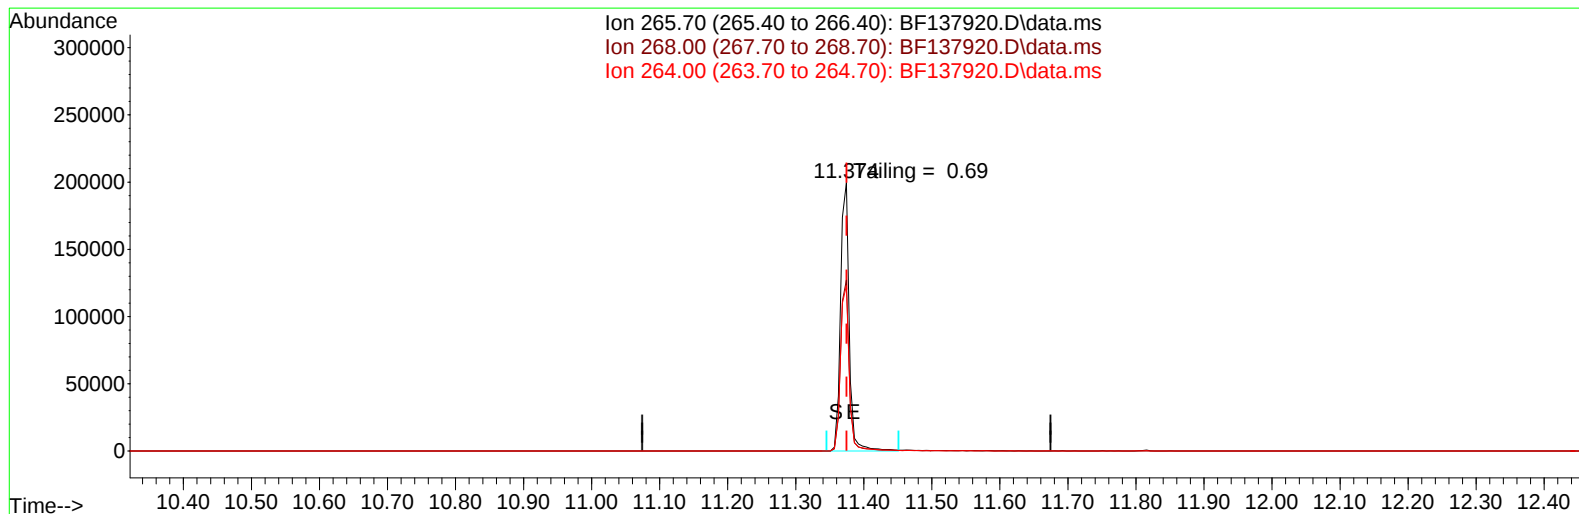

TIC: BF137920.D\data.ms

(70) Pentachlorophenol (C)

11.374min (+ 0.000) 24326.40 ng




response 176478

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.67
264.00	61.80	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051524\
Data File : BF137920.D
Acq On : 15 May 2024 09:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 15 11:34:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

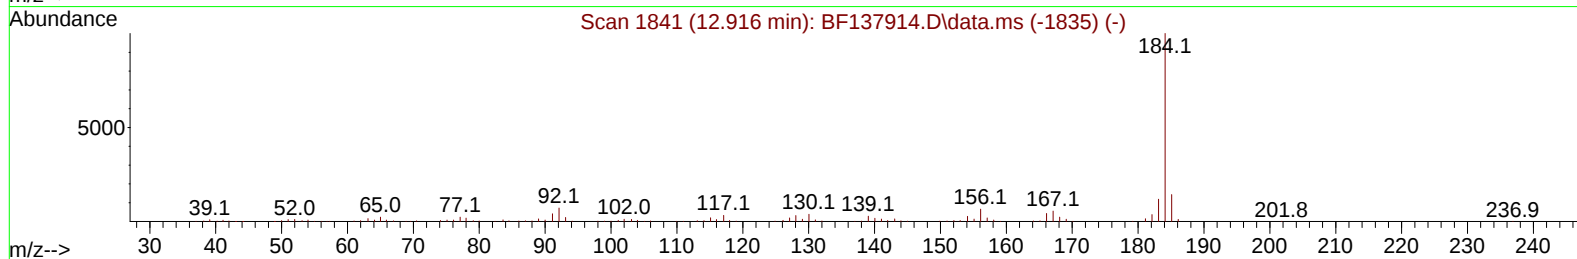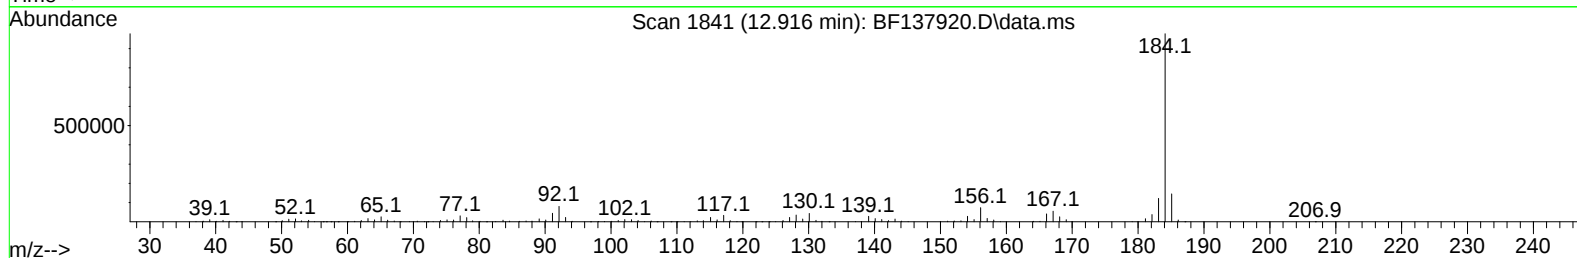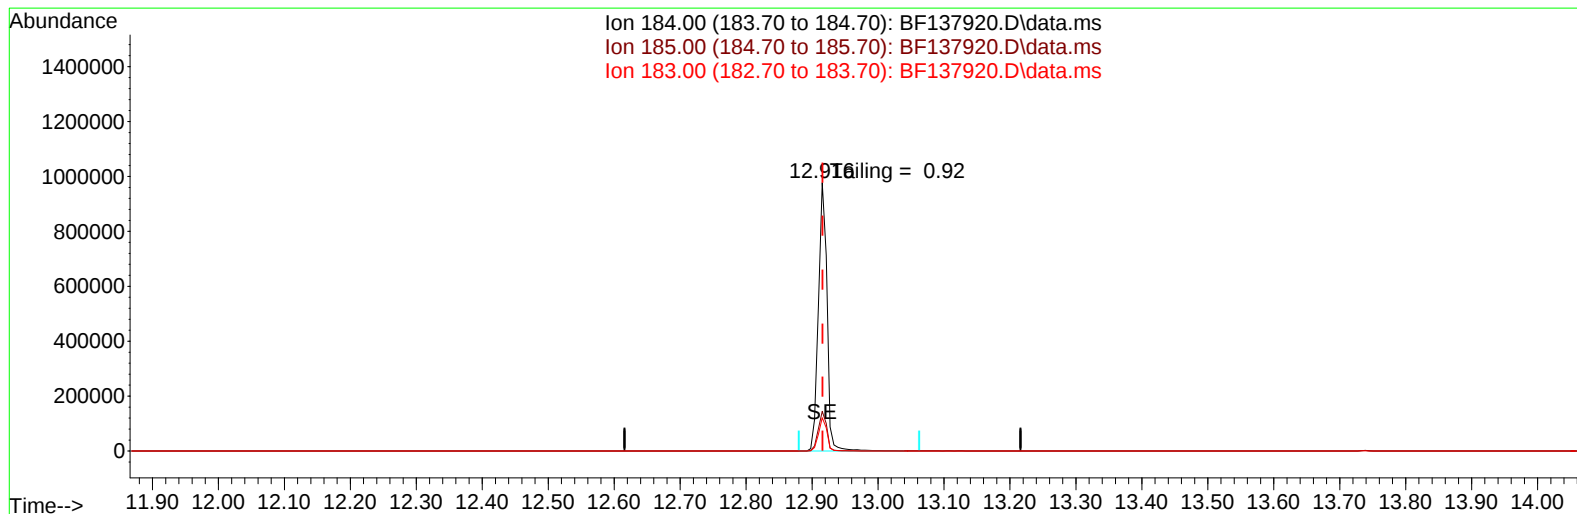

TIC: BF137920.D\data.ms

(77) Benzidine

12.916min (-0.000) 0.00 ng

response 889390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.80
183.00	11.90	12.43
0.00	0.00	0.00