
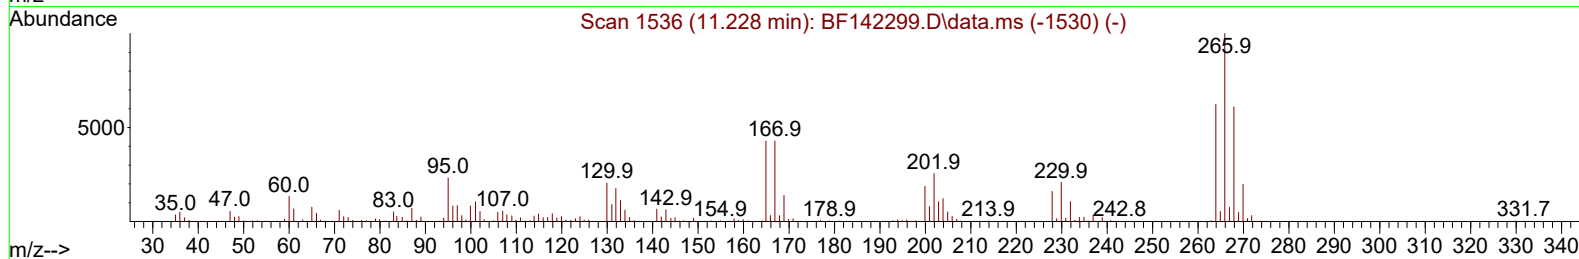
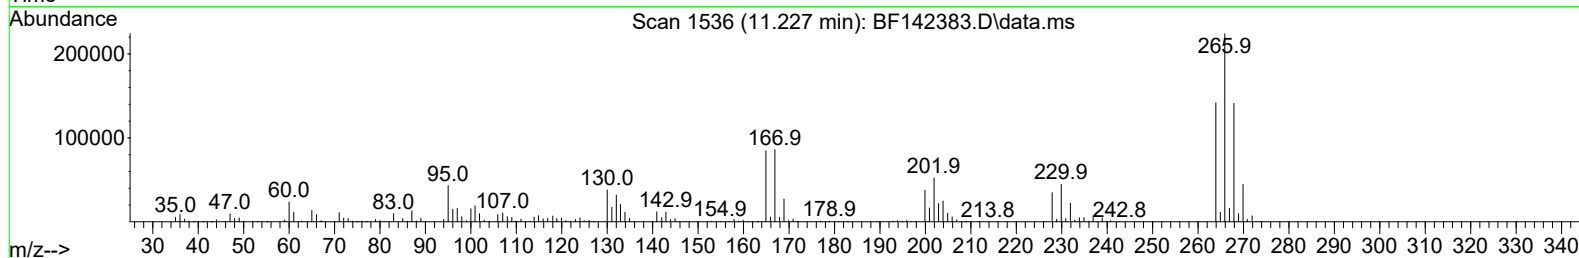


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142383.D
Acq On : 15 May 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:44:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

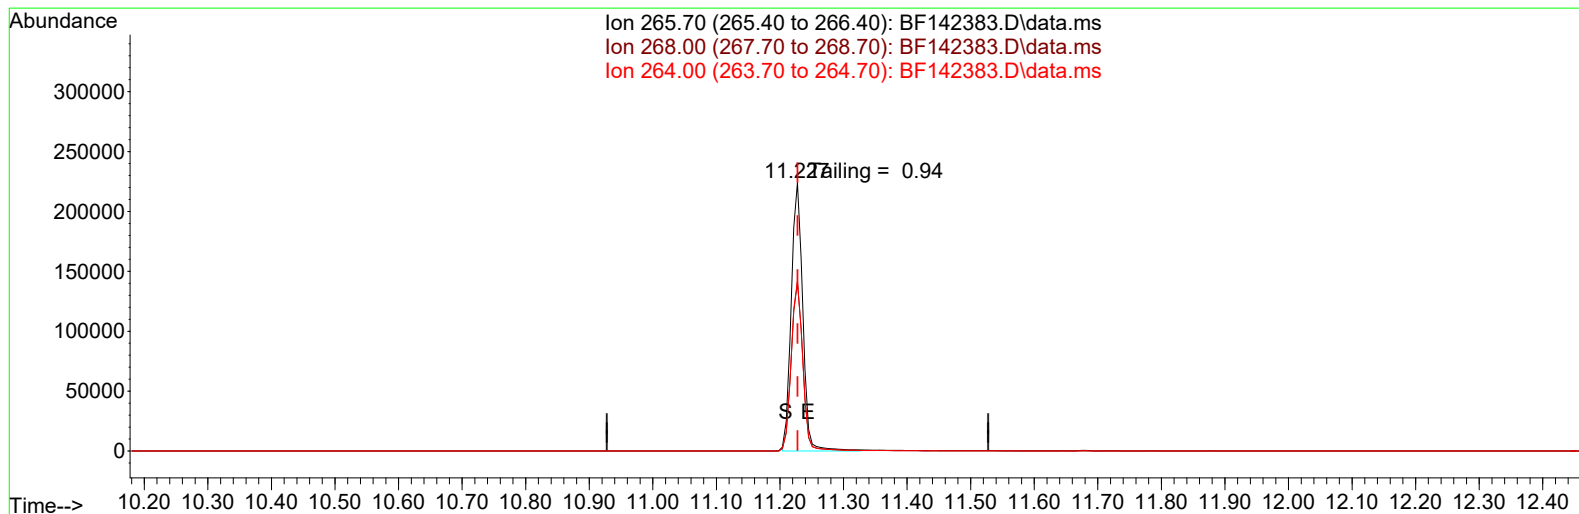

TIC: BF142383.D\data.ms

(70) Pentachlorophenol (C)




11.227min (-0.000) 44844.10 ng

response 288510

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	62.98
264.00	62.20	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142383.D
Acq On : 15 May 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:44:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

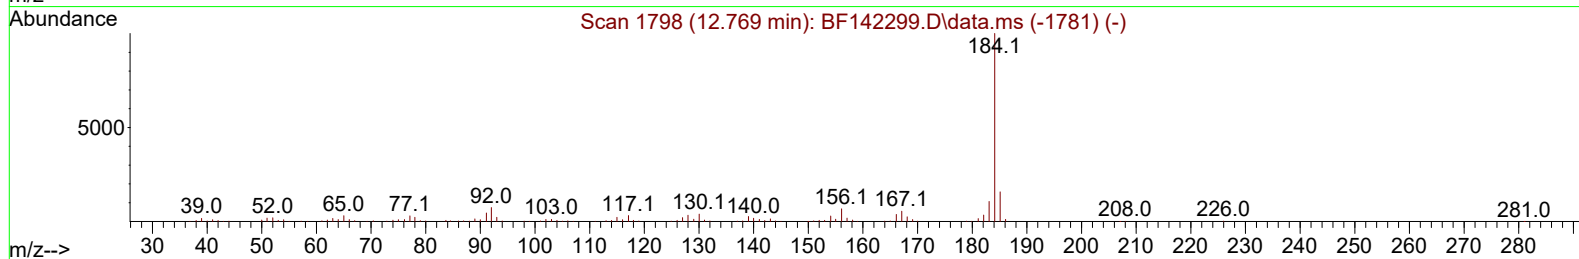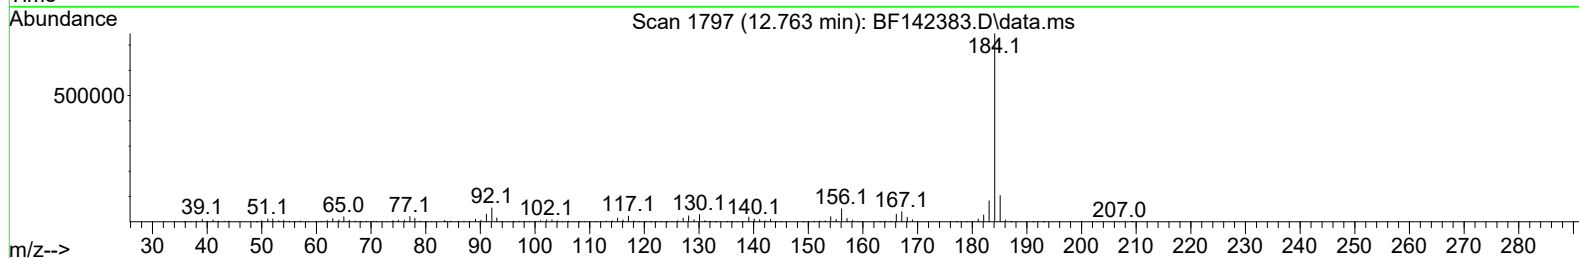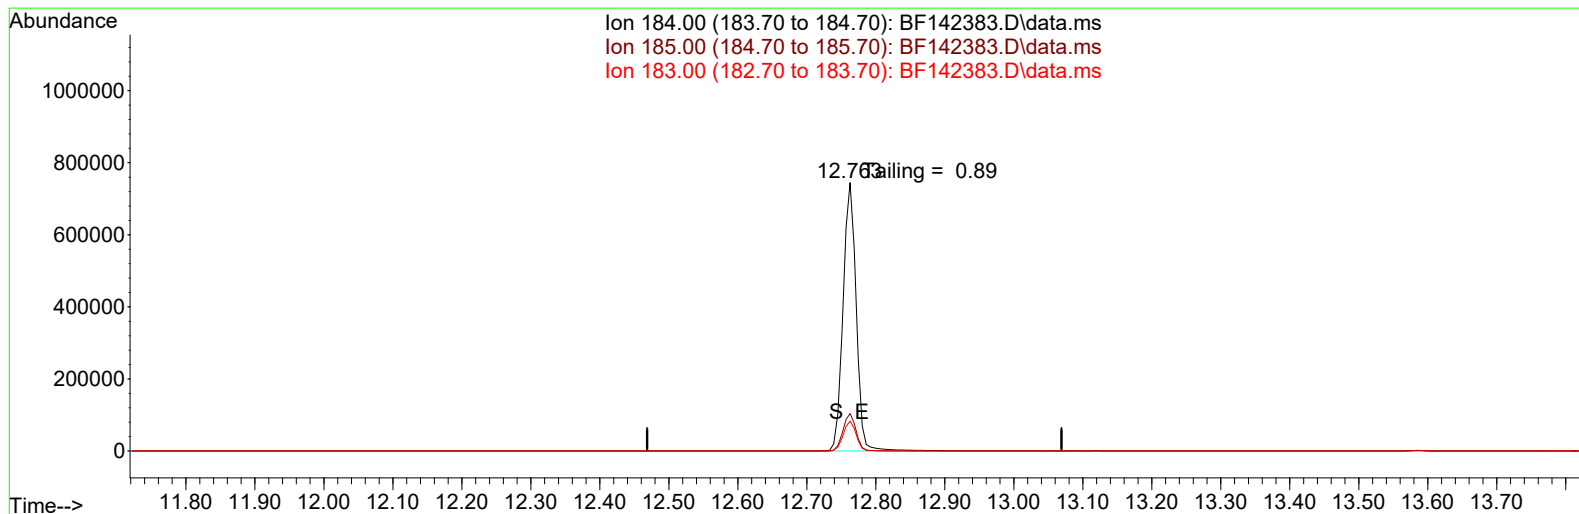

TIC: BF142383.D\data.ms

(77) Benzidine

12.763min (-0.006) 484587.50 ng m

response 977502

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	13.94
183.00	10.70	11.16
0.00	0.00	0.00