
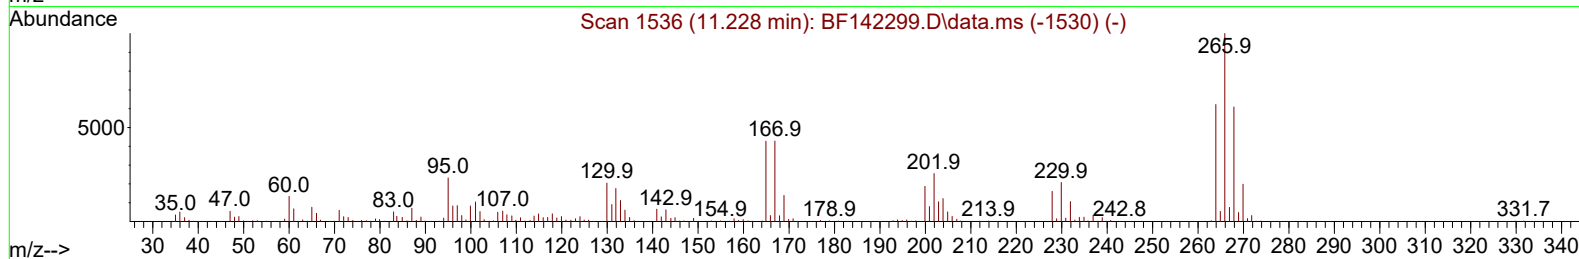
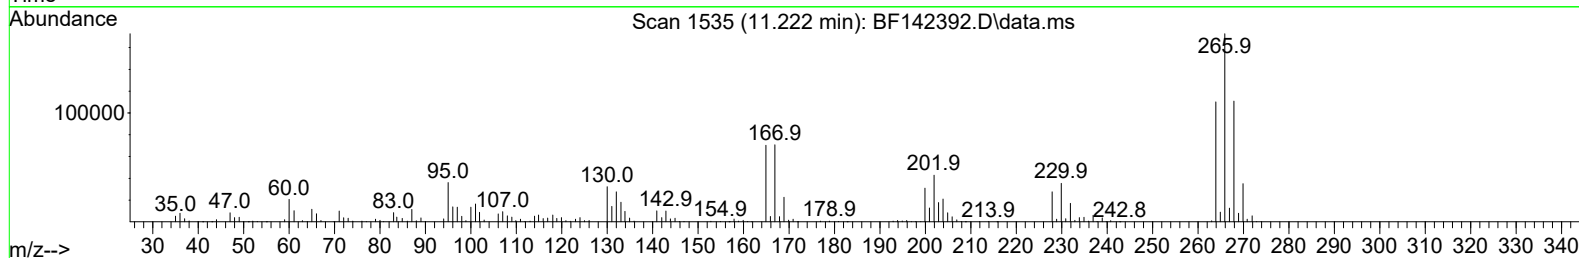


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142392.D
Acq On : 15 May 2025 14:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 04:25:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

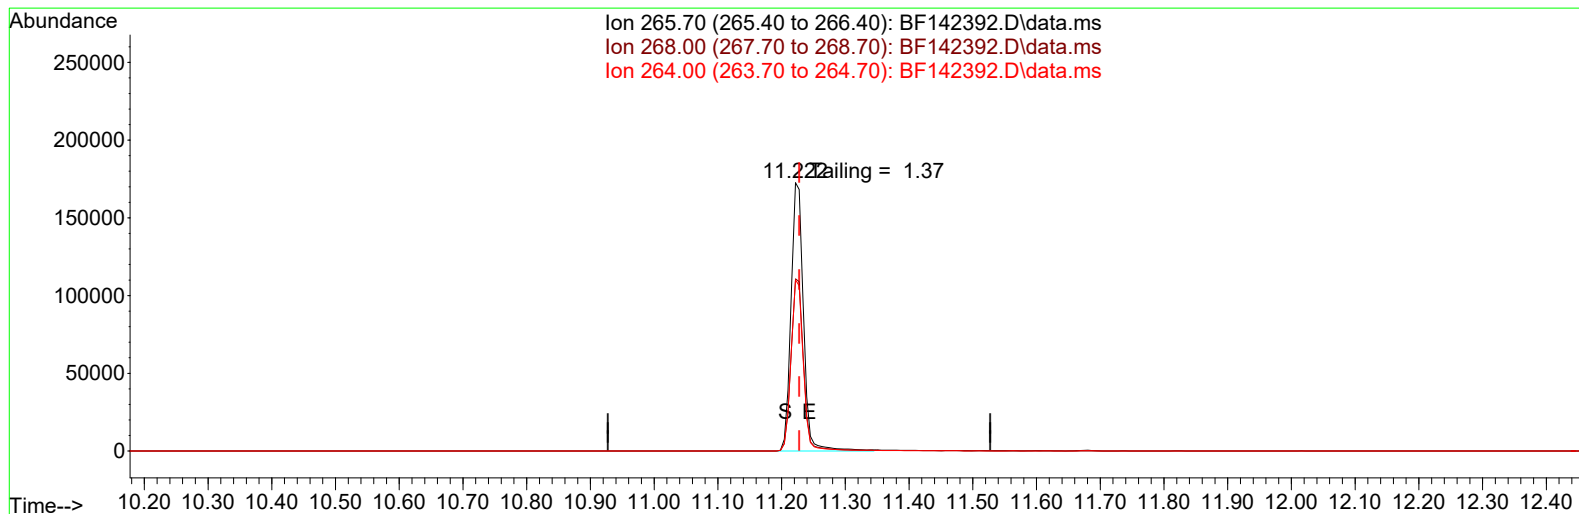

TIC: BF142392.D\data.ms

(70) Pentachlorophenol (C)




11.222min (-0.006) 6218.69 ng

response 238788

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	64.18
264.00	62.20	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142392.D
Acq On : 15 May 2025 14:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 04:25:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

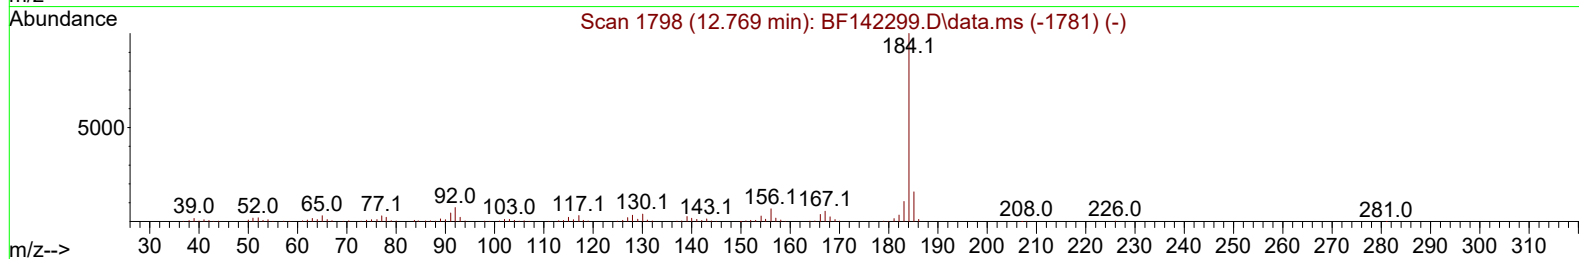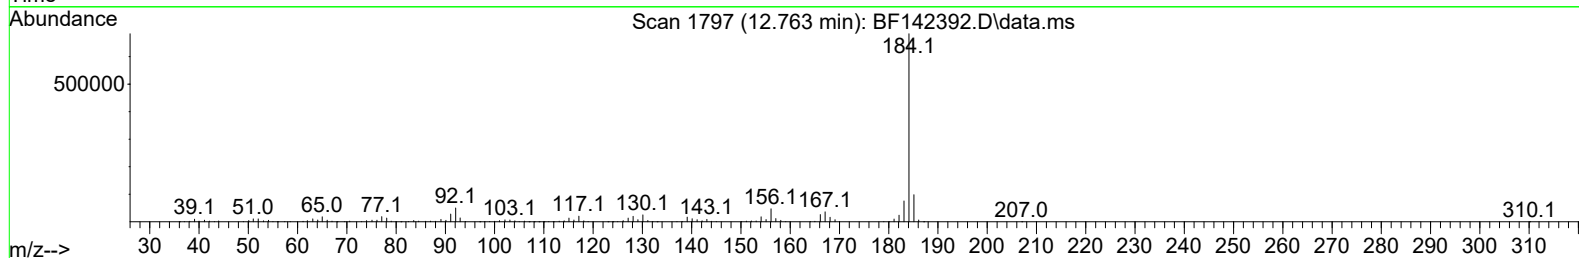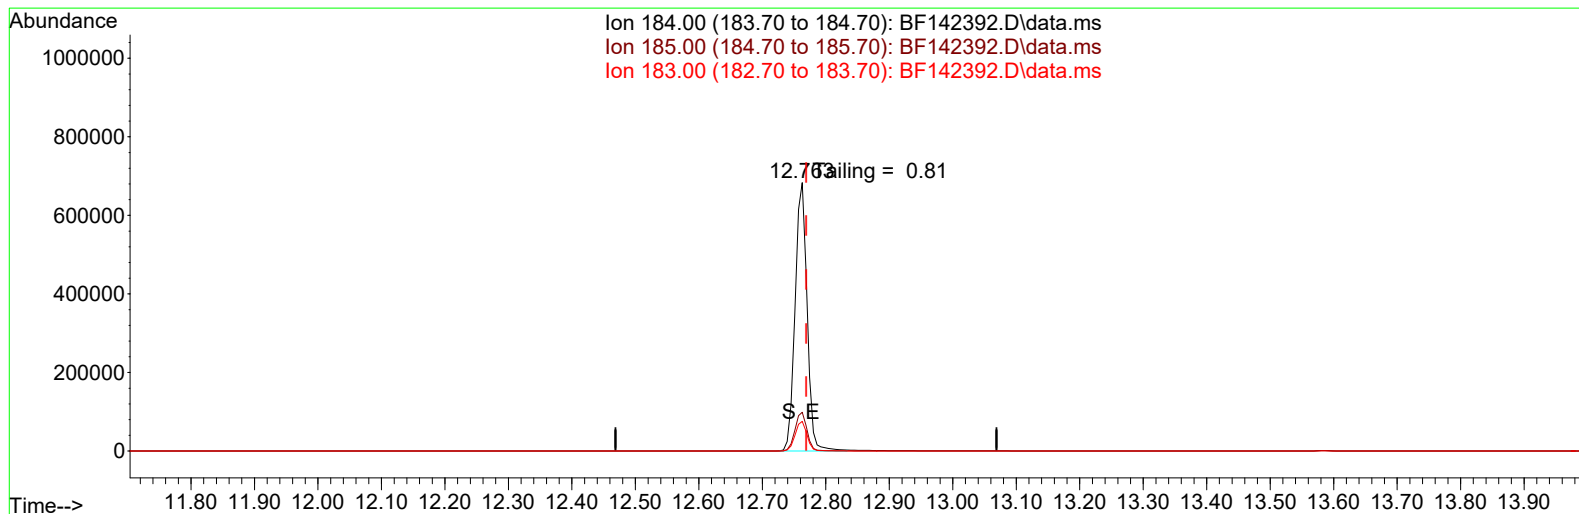

TIC: BF142392.D\data.ms

(77) Benzidine

12.763min (-0.006) 26584.19 ng

response 910179

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.45
183.00	10.70	11.08
0.00	0.00	0.00