

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
 Data File : BF142394.D
 Acq On : 15 May 2025 16:10
 Operator : RC/JU
 Sample : PB167953BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB167953BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.252	3	10	17	rVB	39905	68812	1.35%	0.221%
2	5.140	493	501	511	rVB	276806	460850	9.05%	1.479%
3	5.522	559	566	572	rBV	2897316	4109379	80.71%	13.187%
4	6.522	729	736	741	rBV	2837527	4135768	81.22%	13.272%
5	6.898	795	800	808	rBV	771539	984056	19.33%	3.158%
6	7.298	863	868	876	rBV	37906	52266	1.03%	0.168%
7	7.463	889	896	901	rBV	1896056	2748694	53.98%	8.821%
8	8.181	1012	1018	1030	rBV	989680	1320148	25.93%	4.237%
9	9.257	1194	1201	1206	rBV	3809371	5091745	100.00%	16.340%
10	9.933	1311	1316	1321	rBV	1093822	1436726	28.22%	4.611%
11	10.480	1404	1409	1420	rBV2	36991	51855	1.02%	0.166%
12	10.722	1444	1450	1467	rBV	2222801	3066389	60.22%	9.840%
13	11.422	1564	1569	1577	rBV	1111118	1429258	28.07%	4.587%
14	13.010	1833	1839	1845	rBV	3432781	4547695	89.32%	14.594%
15	14.063	2012	2018	2030	rBV	709575	928731	18.24%	2.980%
16	15.551	2265	2271	2283	rBV	471168	728806	14.31%	2.339%




Sum of corrected areas: 31161178

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142394.D
Acq On : 15 May 2025 16:10
Operator : RC/JU
Sample : PB167953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

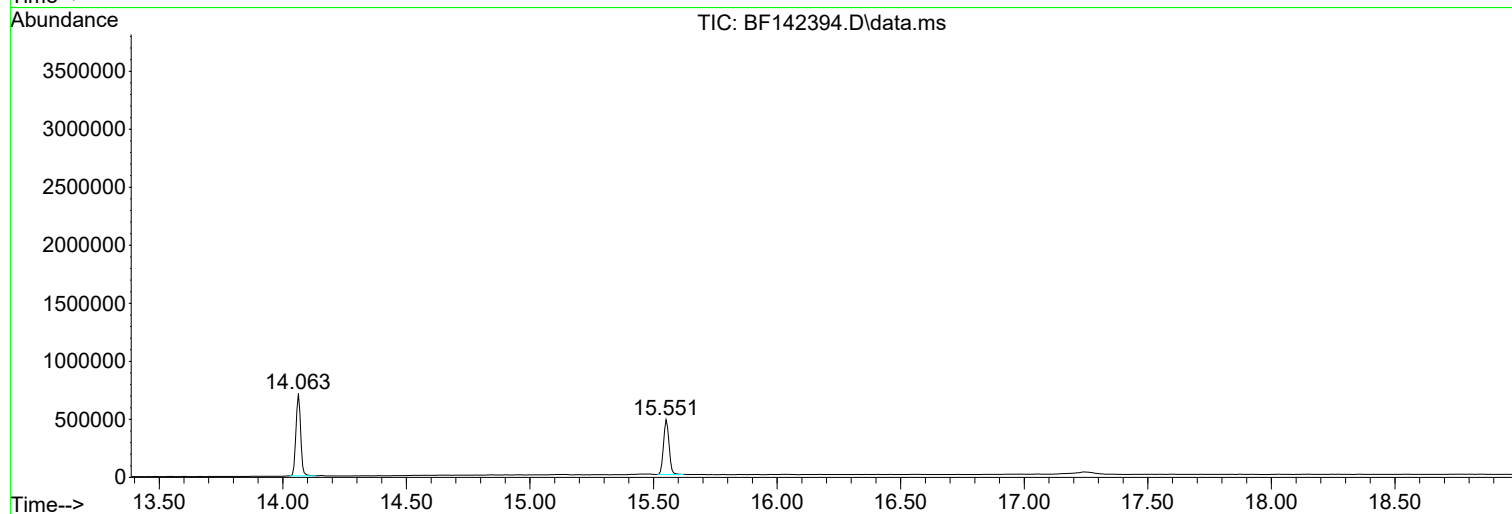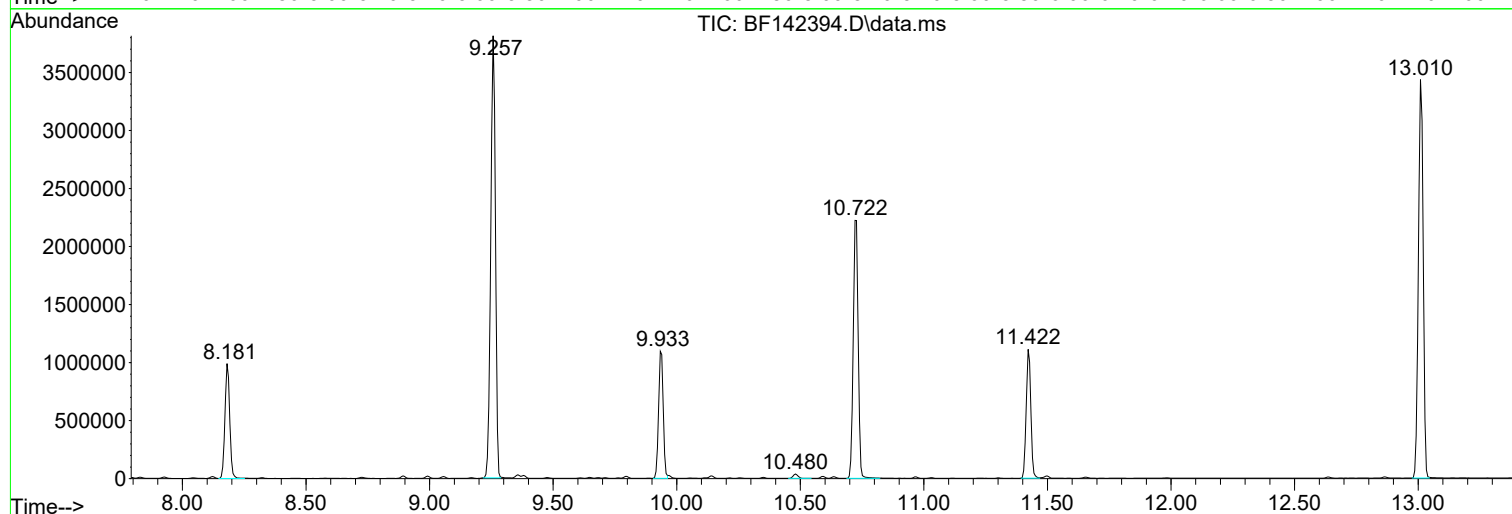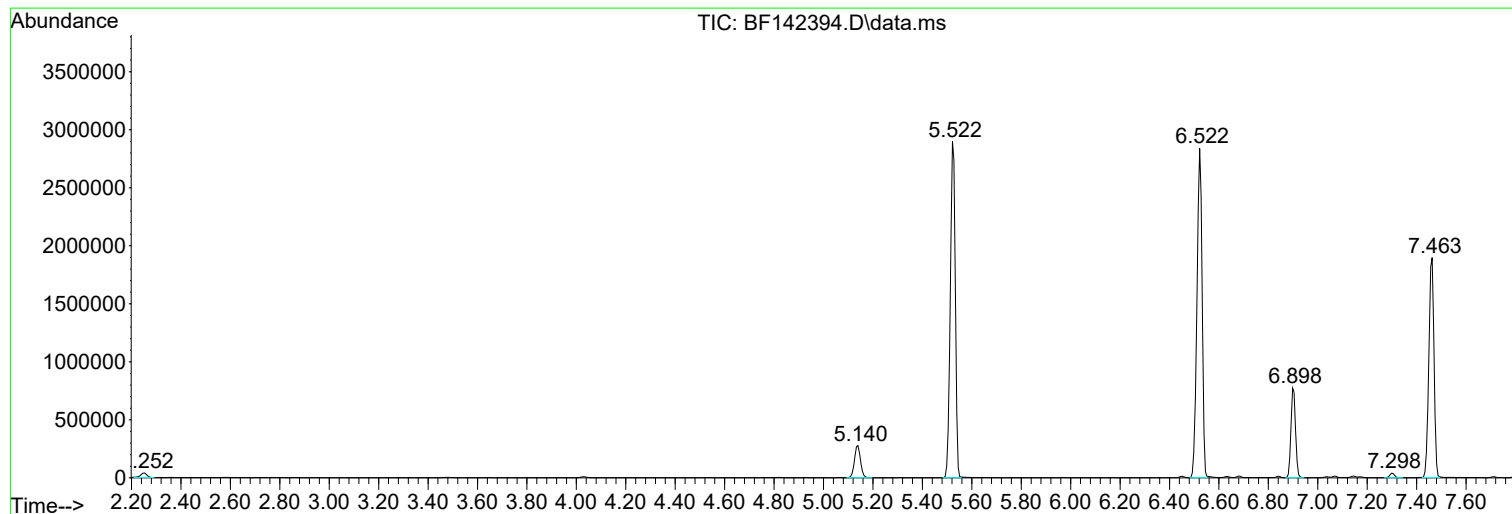

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142394.D
Acq On : 15 May 2025 16:10
Operator : RC/JU
Sample : PB167953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB167953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
5.140	9.37 ng	460850	1,4-Dichlorobenzene-d4			6.898
Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59	
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16	
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12	
4	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	9	
5	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	9	

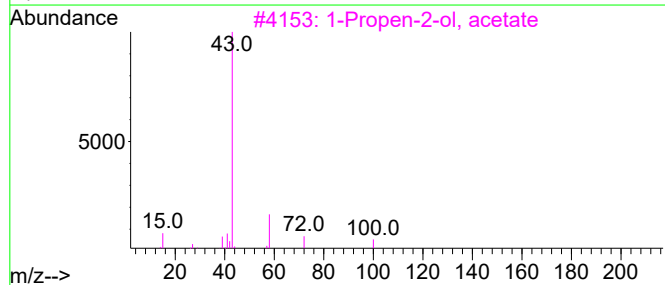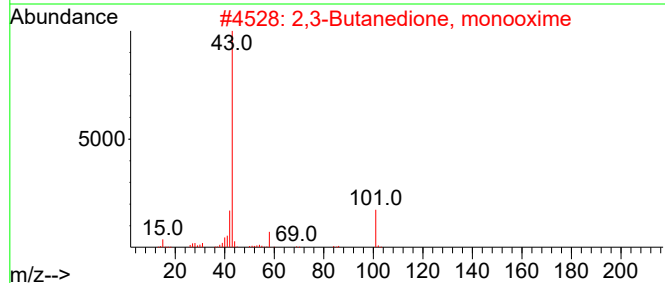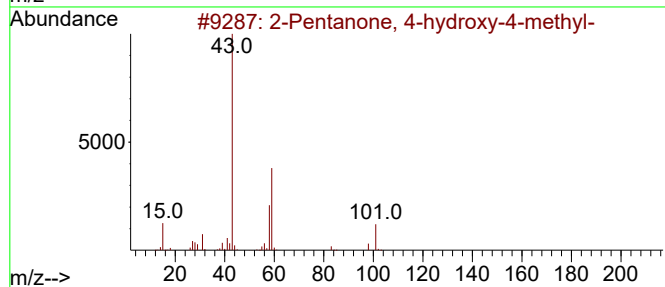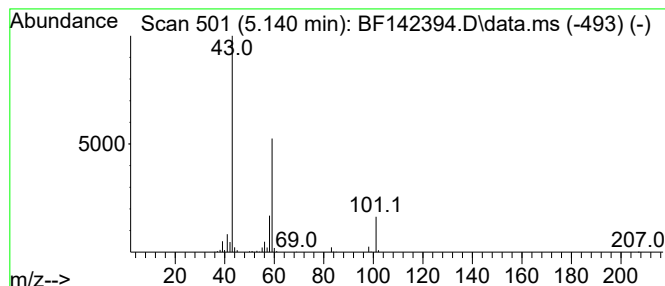

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142394.D
Acq On : 15 May 2025 16:10
Operator : RC/JU
Sample : PB167953BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167953BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.140	9.4	ng	460850	1	6.898	984056	20.0