
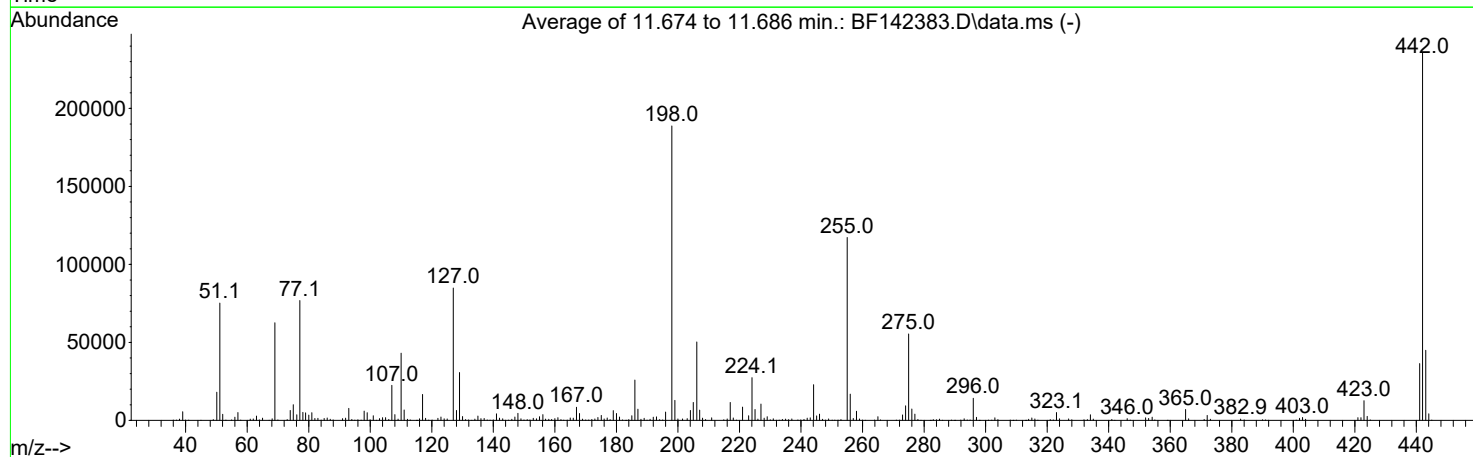


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142383.D
Acq On : 15 May 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 05 18:41:44 2025

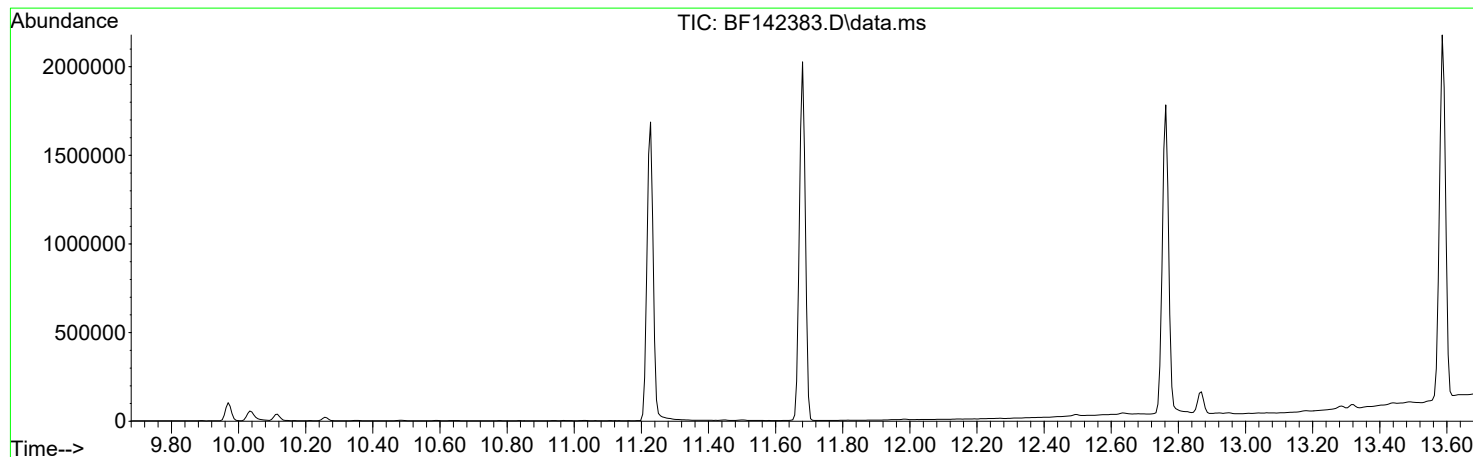

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	75184	PASS
68	69	0.00	2	1.7	1079	PASS
69	198	0.00	100	33.2	62629	PASS
70	69	0.00	2	0.5	299	PASS
127	198	10	80	45.0	84867	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	188736	PASS
199	198	5	9	6.8	12787	PASS
275	198	10	60	29.3	55387	PASS
365	198	1	100	3.7	6961	PASS
441	198	0.01	100	19.3	36435	PASS
442	442	50	100	100.0	235861	PASS
443	442	15	24	19.1	44984	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/15/2025	BNA_F	<u>BF142383.D</u>
Compound Name	Response	Retention Time
DDT	530900	13.586
DDD	9628	13.321
DDE	972	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10600	541500	1.96

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142383.D
Acq On : 15 May 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 16 03:44:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

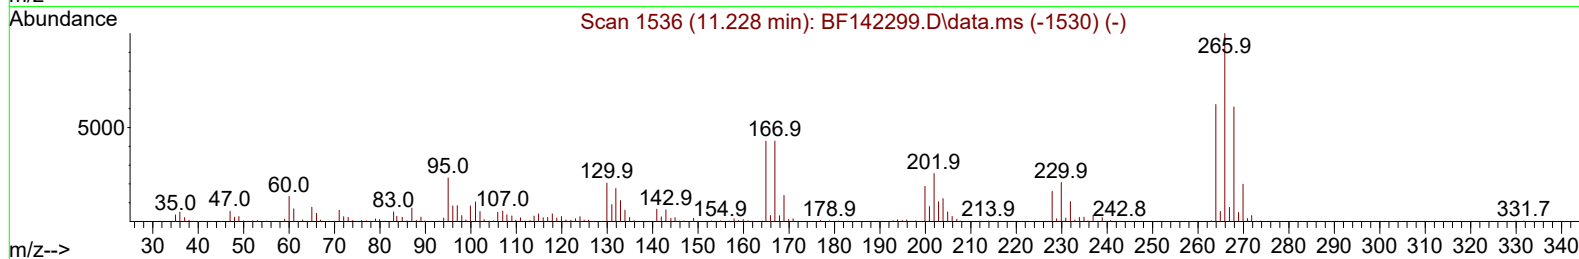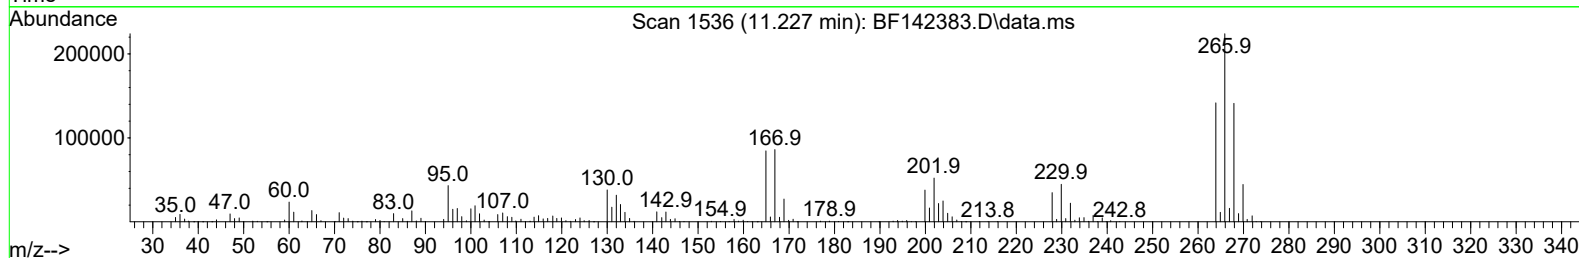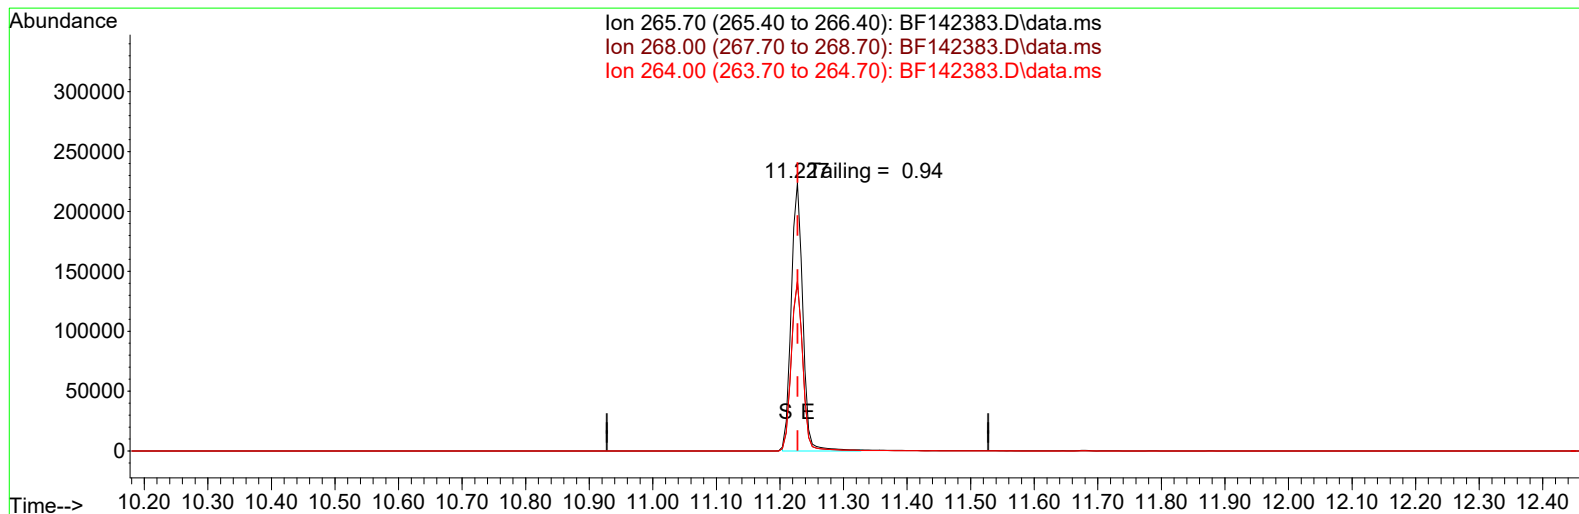

TIC: BF142383.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 44844.10 ng




response 288510

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	62.98
264.00	62.20	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051525\
Data File : BF142383.D
Acq On : 15 May 2025 09:09
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 16 03:44:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

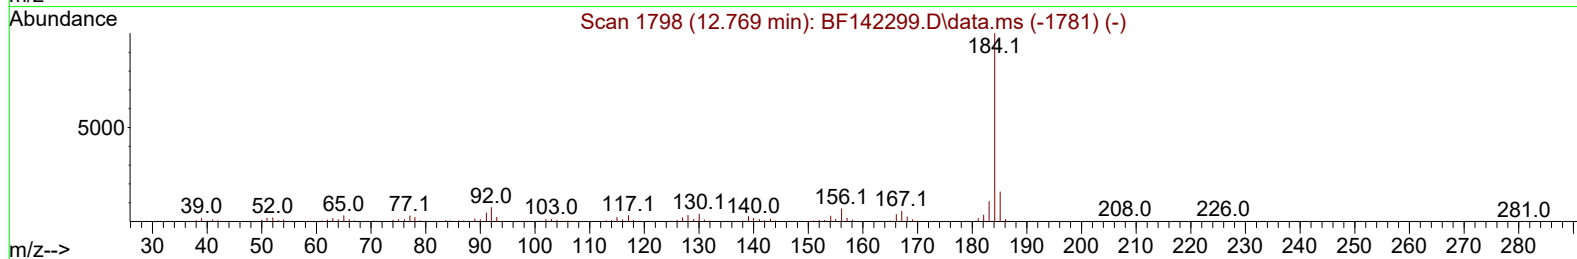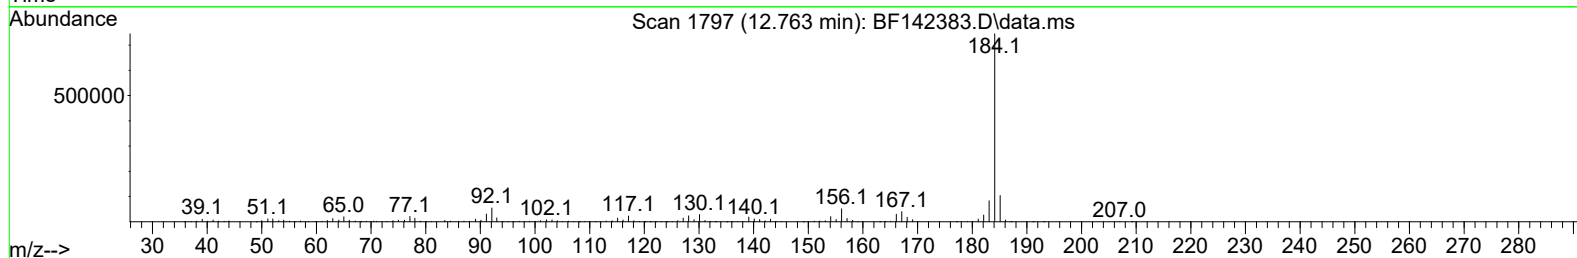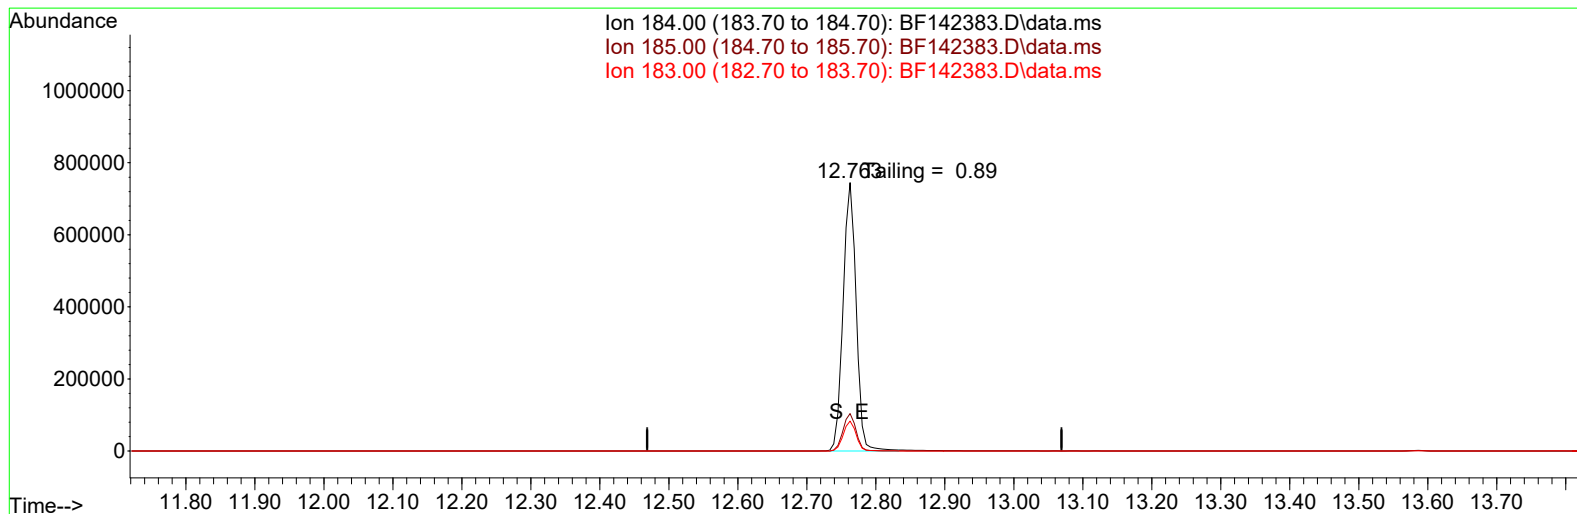

TIC: BF142383.D\data.ms

(77) Benzidine

12.763min (-0.006) 484587.50 ng m

response 977502

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	13.94
183.00	10.70	11.16
0.00	0.00	0.00