
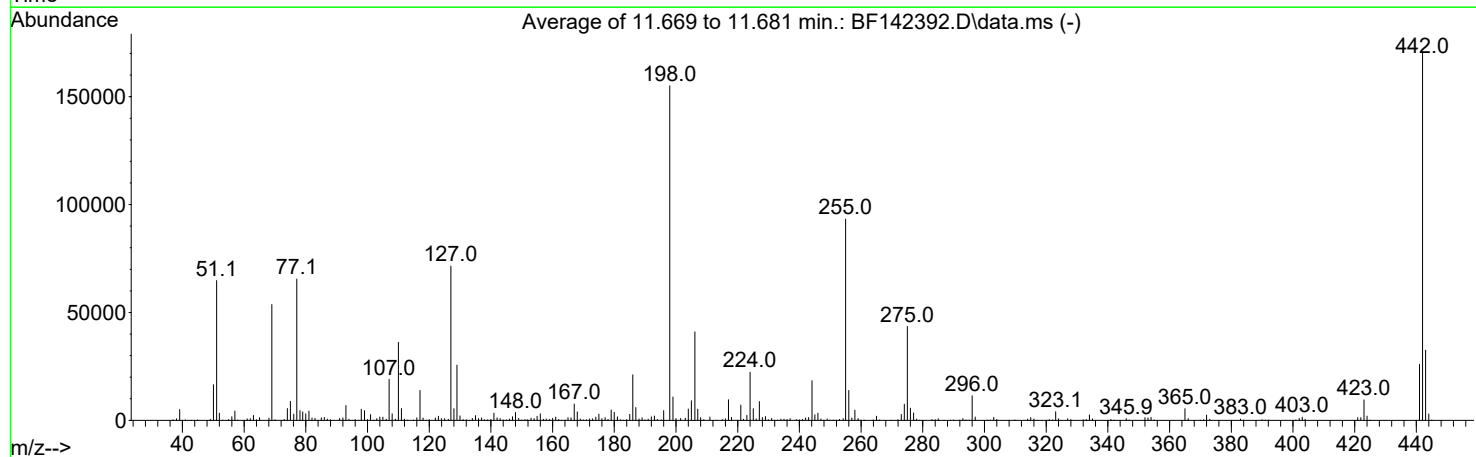


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051525\  
Data File : BF142392.D  
Acq On : 15 May 2025 14:27  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050525.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Mon May 05 18:41:44 2025

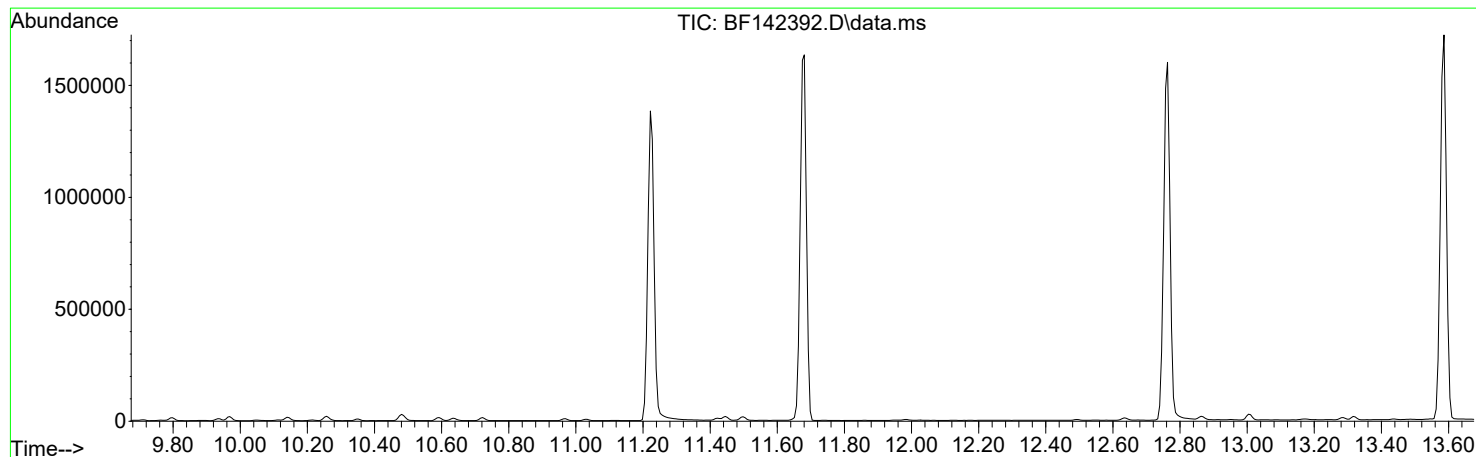

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.8         | 64813      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 1009       | PASS                |
| 69             | 198             | 0.00            | 100             | 34.6         | 53688      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 289        | PASS                |
| 127            | 198             | 10              | 80              | 46.1         | 71499      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 155067     | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 10803      | PASS                |
| 275            | 198             | 10              | 60              | 28.1         | 43517      | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 5444       | PASS                |
| 441            | 198             | 0.01            | 100             | 16.8         | 25998      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 170453     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 32579      | PASS                |

# DDT Breakdown


| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 5/15/2025     | BNA_F            | <u>BF142392.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 450840           | 13.586             |
| DDD           | 7184             | 13.316             |
| DDE           | 494              | 12.951             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7678          | 458518           | 1.67               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051525\  
Data File : BF142392.D  
Acq On : 15 May 2025 14:27  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 16 04:25:11 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 05 18:41:44 2025  
Response via : Initial Calibration

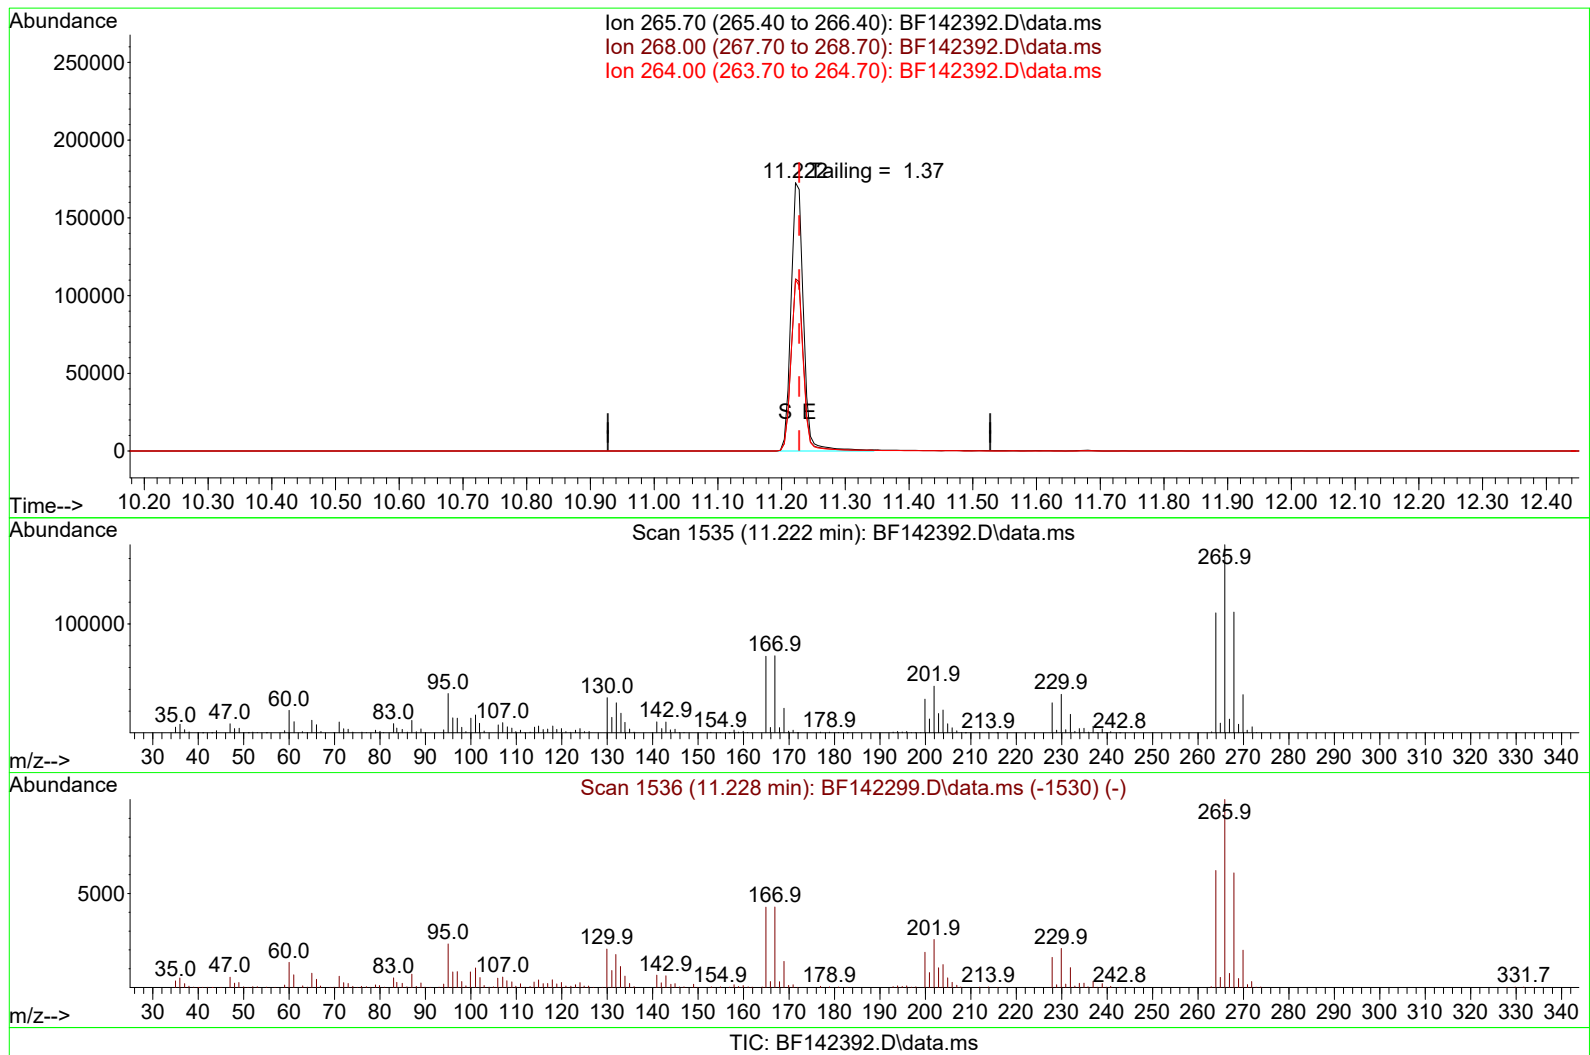

(70) Pentachlorophenol (C)

11.222min (-0.006) 6218.69 ng




response 238788

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 60.90  | 64.18  |
| 264.00 | 62.20  | 63.82  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051525\  
Data File : BF142392.D  
Acq On : 15 May 2025 14:27  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: May 16 04:25:11 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF050525.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 05 18:41:44 2025  
Response via : Initial Calibration

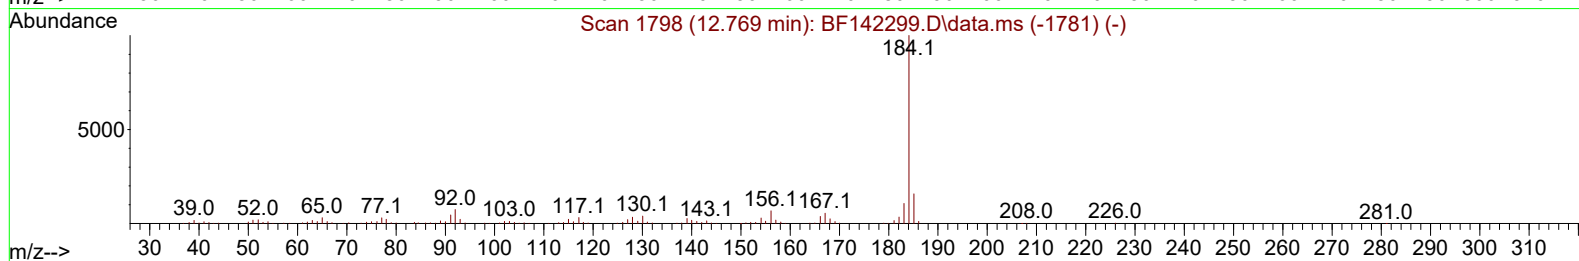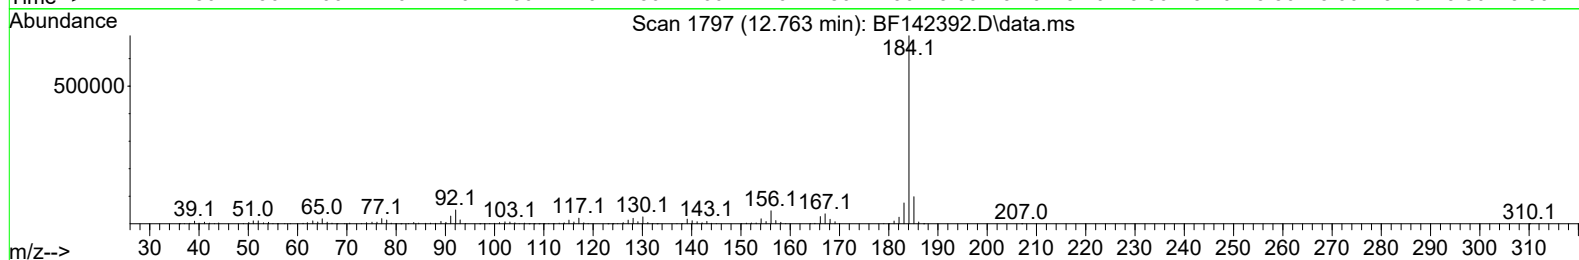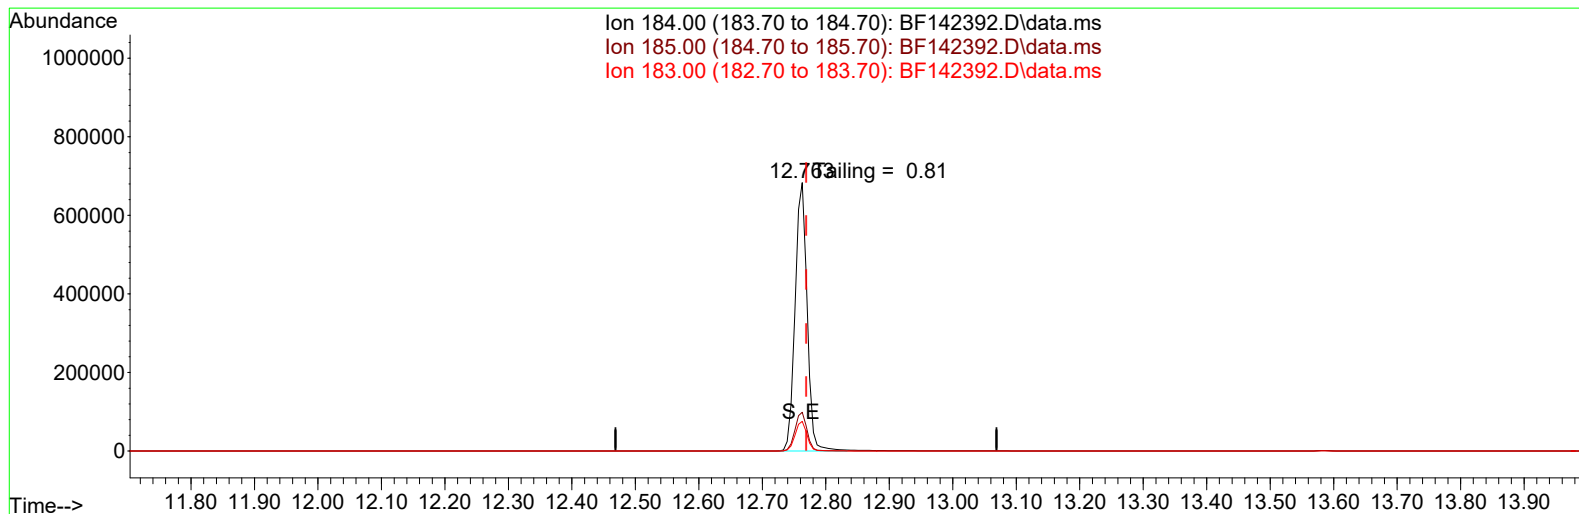

TIC: BF142392.D\data.ms

**(77) Benzidine**

**12.763min (-0.006) 26584.19 ng**

**response 910179**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.70  | 14.45  |
| 183.00 | 10.70  | 11.08  |
| 0.00   | 0.00   | 0.00   |