


Data Path : Z:\HPCHEM1\BNA F\Data\BF051616\
 Data File : BF087074.D
 Acq On : 16 May 2016 11:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 17 10:57:13 2016

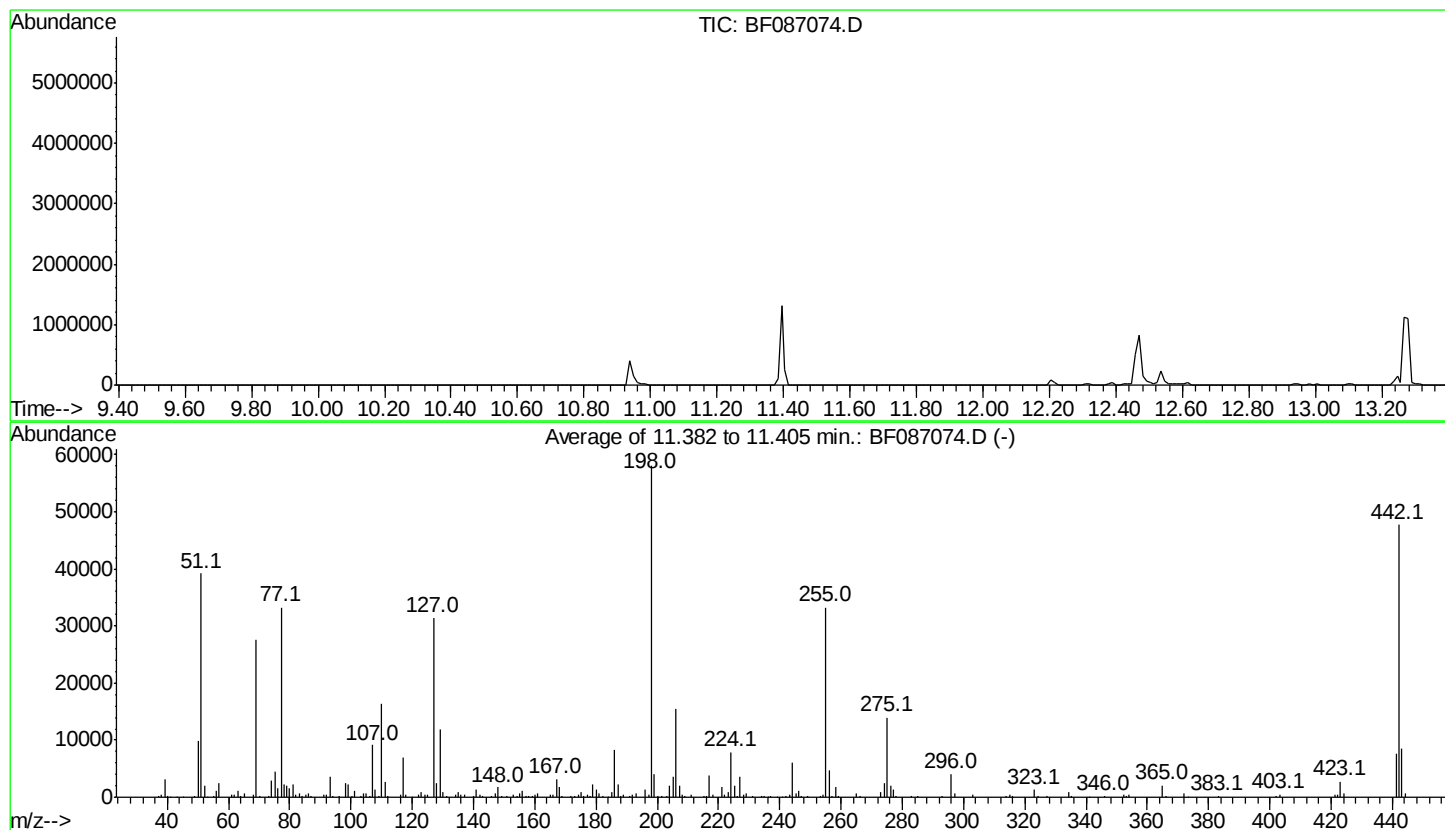

AutoFind: Scans 857, 858, 859; Background Corrected with Scan 854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.4	39149	PASS
68	69	0.00	2	1.7	469	PASS
69	198	0.00	100	47.6	27644	PASS
70	69	0.00	2	0.5	140	PASS
127	198	10	80	54.2	31490	PASS
197	198	0.00	2	0.8	437	PASS
198	198	100	100	100.0	58075	PASS
199	198	5	9	7.1	4112	PASS
275	198	10	60	24.0	13955	PASS
365	198	1	100	3.5	2022	PASS
441	442	0.01	24	16.0	7642	PASS
442	198	50	100	82.2	47746	PASS
443	442	15	24	18.0	8612	PASS