


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051617\
 Data File : BF095157.D
 Acq On : 16 May 2017 15:24
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 03 17:24:51 2017

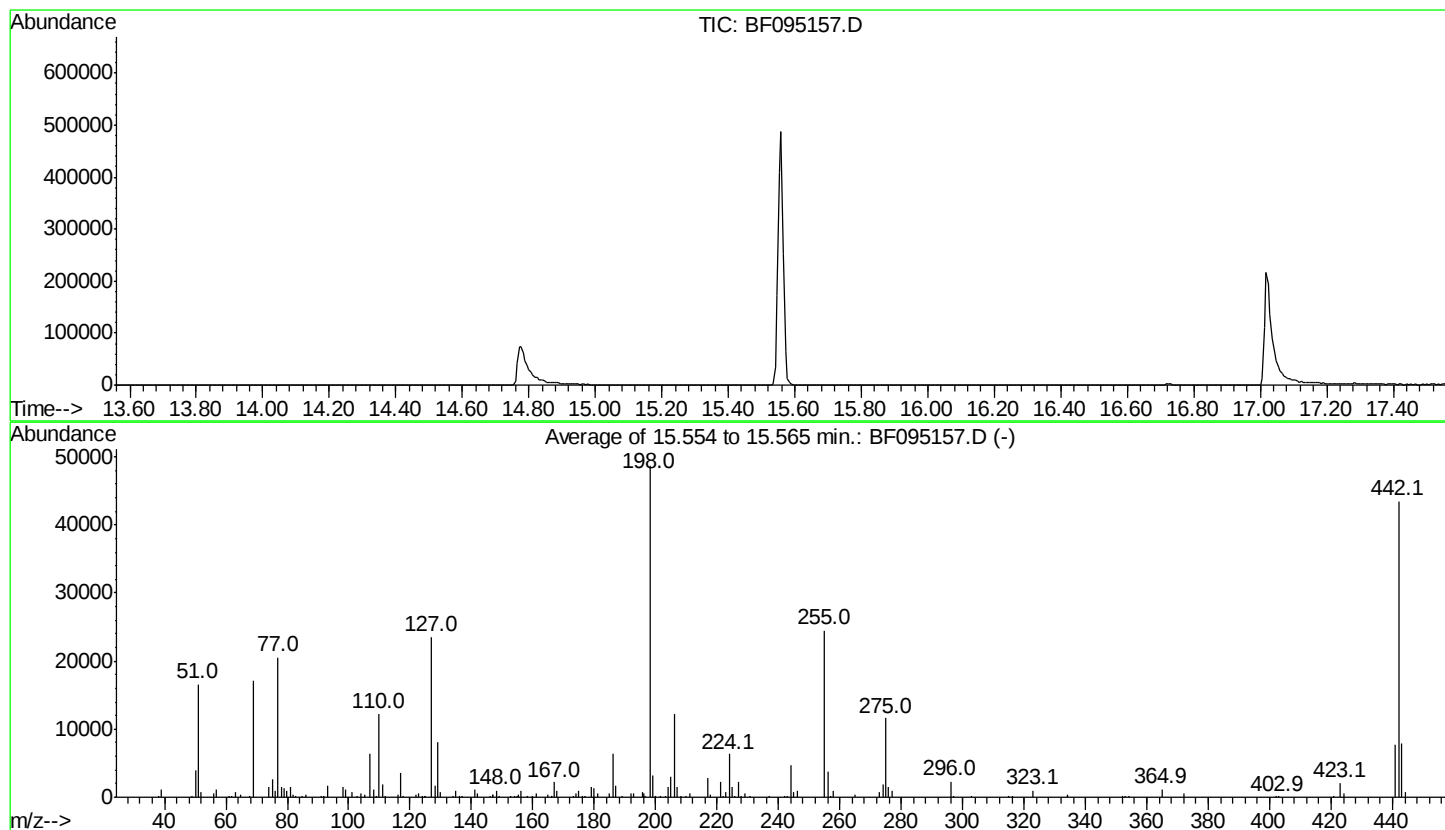

AutoFind: Scans 2315, 2316, 2317; Background Corrected with Scan 2309

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	16611	PASS
68	69	0.00	2	1.1	192	PASS
69	198	0.00	100	35.0	17025	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	23517	PASS
197	198	0.00	2	0.3	163	PASS
198	198	100	100	100.0	48698	PASS
199	198	5	9	6.4	3130	PASS
275	198	10	60	23.9	11615	PASS
365	198	1	100	2.4	1147	PASS
441	442	0.01	24	17.5	7621	PASS
442	198	50	100	89.2	43440	PASS
443	442	15	24	18.4	7976	PASS