


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051617\
Data File : BF095179.D
Acq On : 17 May 2017 4:01
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 03 17:24:51 2017

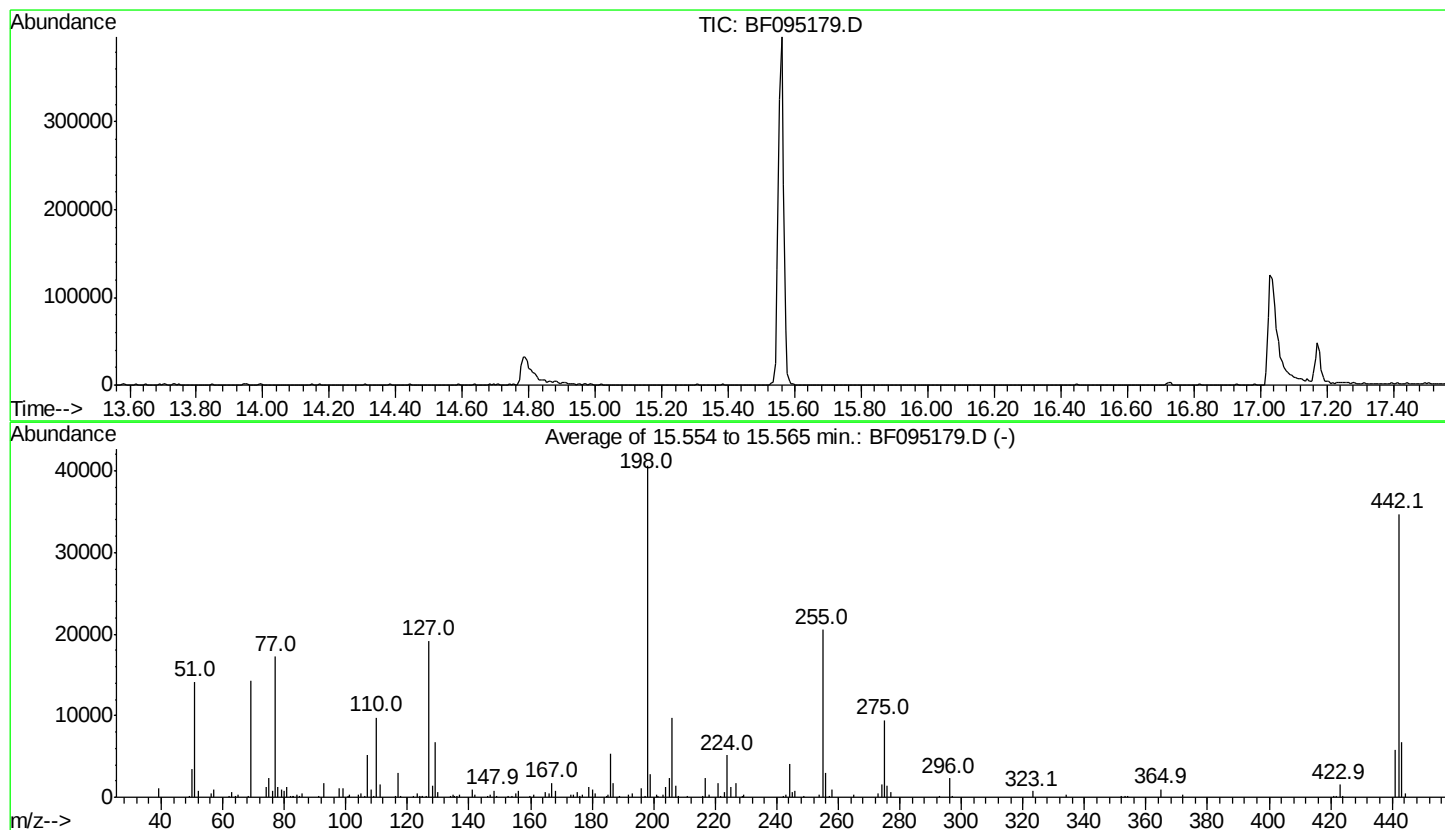

AutoFind: Scans 2315, 2316, 2317; Background Corrected with Scan 2310

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	14172	PASS
68	69	0.00	2	1.6	233	PASS
69	198	0.00	100	35.1	14274	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	19208	PASS
197	198	0.00	2	0.6	232	PASS
198	198	100	100	100.0	40650	PASS
199	198	5	9	7.1	2872	PASS
275	198	10	60	23.2	9440	PASS
365	198	1	100	2.5	1000	PASS
441	442	0.01	24	16.6	5773	PASS
442	198	50	100	85.5	34754	PASS
443	442	15	24	19.6	6812	PASS