


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051619\
 Data File : BF114302.D
 Acq On : 16 May 2019 10:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 10 15:56:46 2019

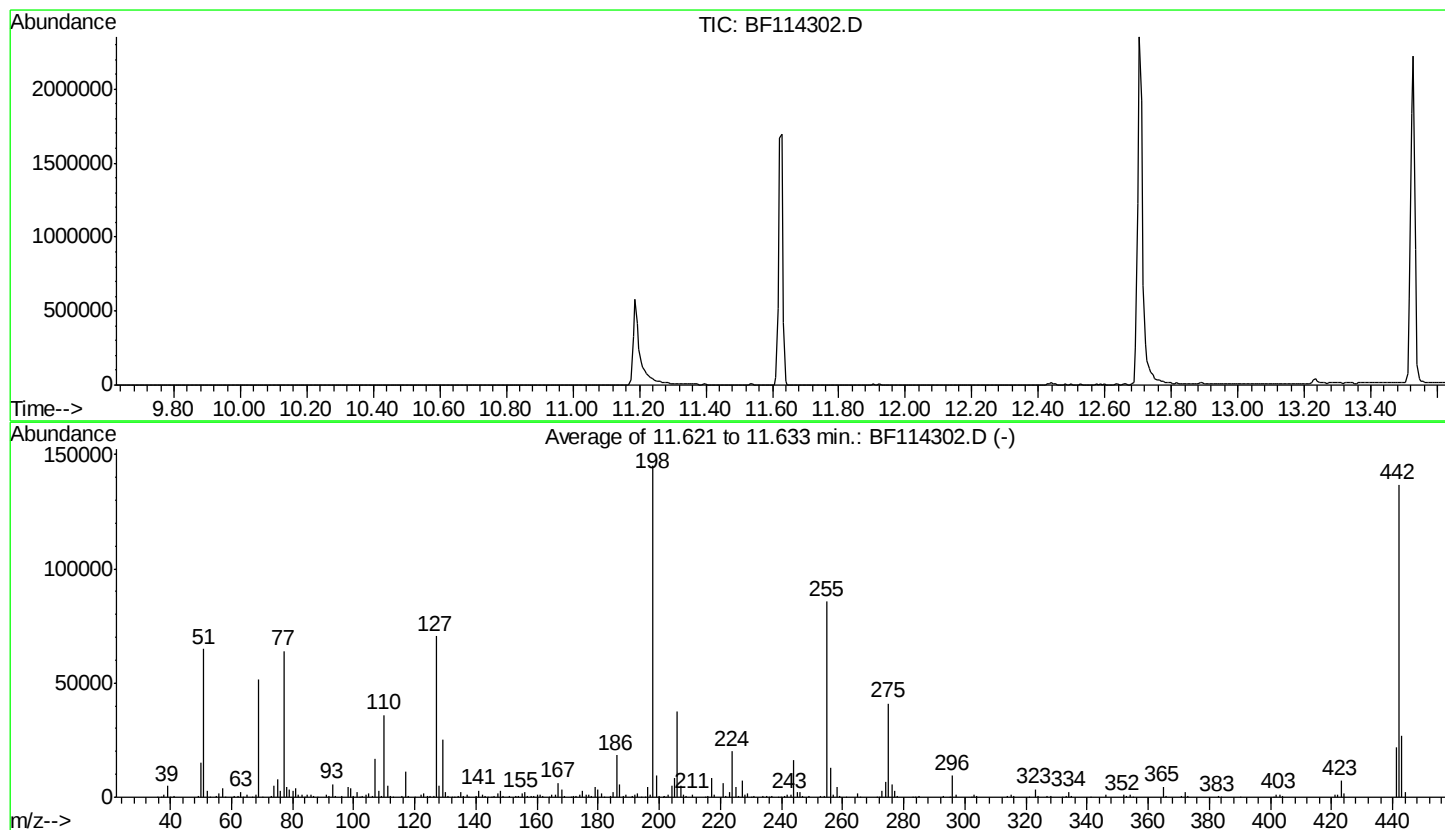

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	64750	PASS
68	69	0.00	2	1.8	912	PASS
69	198	0.00	100	35.7	51789	PASS
70	69	0.00	2	0.3	132	PASS
127	198	10	80	48.5	70421	PASS
197	198	0.00	2	0.7	949	PASS
198	198	100	100	100.0	145157	PASS
199	198	5	9	6.6	9556	PASS
275	198	10	60	28.2	40998	PASS
365	198	1	100	3.2	4648	PASS
441	198	0.01	100	15.0	21846	PASS
442	198	50	100	94.4	136984	PASS
443	442	15	24	19.8	27128	PASS