


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF051619\  
 Data File : BF114325.D  
 Acq On : 16 May 2019 23:18  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri May 10 15:56:46 2019

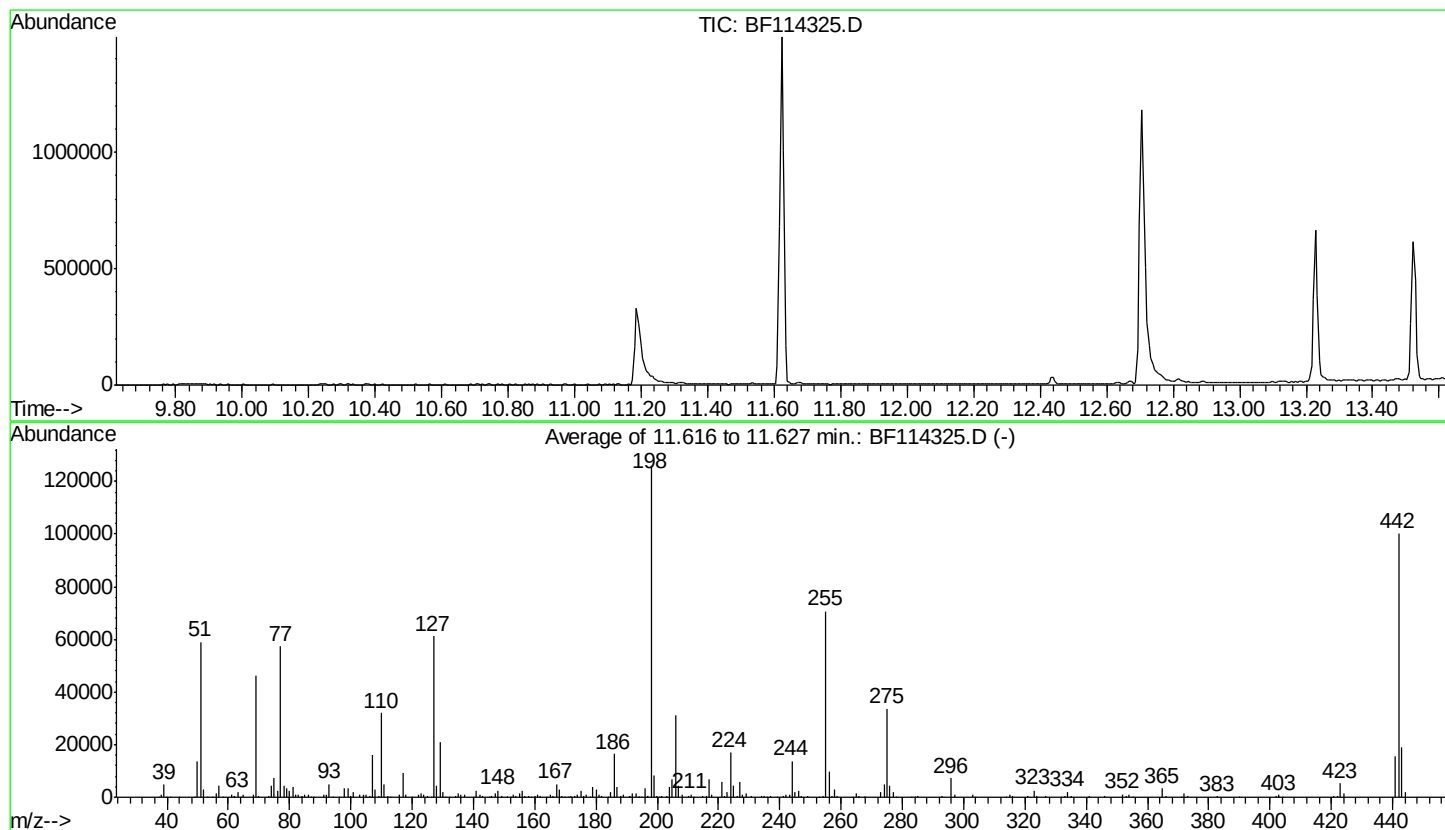

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1616

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 46.8      | 58973   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 806     | PASS             |
| 69          | 198          | 0.00         | 100          | 36.8      | 46344   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.8       | 373     | PASS             |
| 127         | 198          | 10           | 80           | 48.6      | 61221   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 518     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 126032  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 8416    | PASS             |
| 275         | 198          | 10           | 60           | 26.8      | 33794   | PASS             |
| 365         | 198          | 1            | 100          | 2.7       | 3355    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.2      | 15423   | PASS             |
| 442         | 198          | 50           | 100          | 79.5      | 100197  | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 19203   | PASS             |