

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
 Data File : BF128264.D
 Acq On : 16 May 2022 13:10
 Operator : CG\JU
 Sample : N2852-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	544	547	565	rBV	808329	729441	25.86%	4.556%
2	6.510	715	718	731	rBV	535339	469391	16.64%	2.932%
3	6.881	778	781	785	rBV	981367	873233	30.95%	5.454%
4	7.451	873	878	881	rBV	1645687	1559119	55.26%	9.738%
5	8.169	995	1000	1003	rBV	1257884	1089794	38.63%	6.807%
6	9.245	1177	1183	1186	rBV	2929319	2649347	93.91%	16.548%
7	9.928	1294	1299	1302	rBV	1433276	1256532	44.54%	7.848%
8	10.716	1429	1433	1444	rBV	1384886	1176164	41.69%	7.346%
9	11.416	1548	1552	1556	rBV	1530782	1348934	47.81%	8.426%
10	13.004	1817	1822	1825	rBV	3249822	2821184	100.00%	17.621%
11	13.904	1970	1975	1985	rBV10	17593	50886	1.80%	0.318%
12	14.063	1998	2002	2006	rBV	1208843	1086872	38.53%	6.789%
13	14.151	2013	2017	2023	rBV	30325	33167	1.18%	0.207%
14	15.557	2250	2256	2267	rVB	670862	865985	30.70%	5.409%




Sum of corrected areas: 16010049

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128264.D
Acq On : 16 May 2022 13:10
Operator : CG\JU
Sample : N2852-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

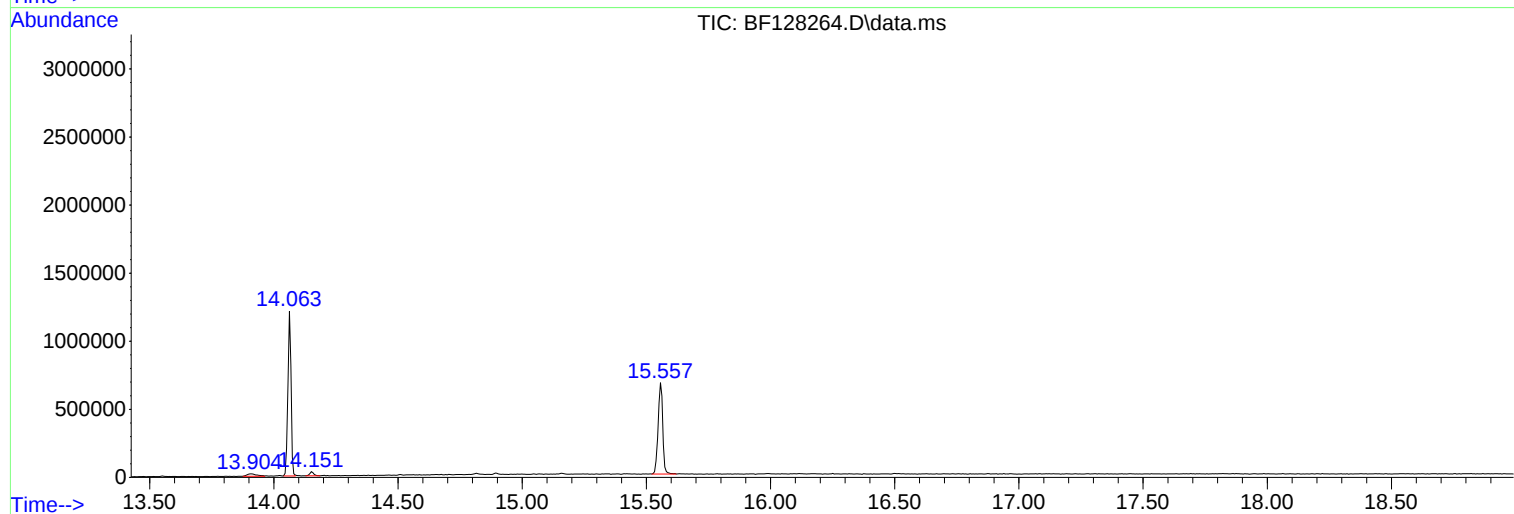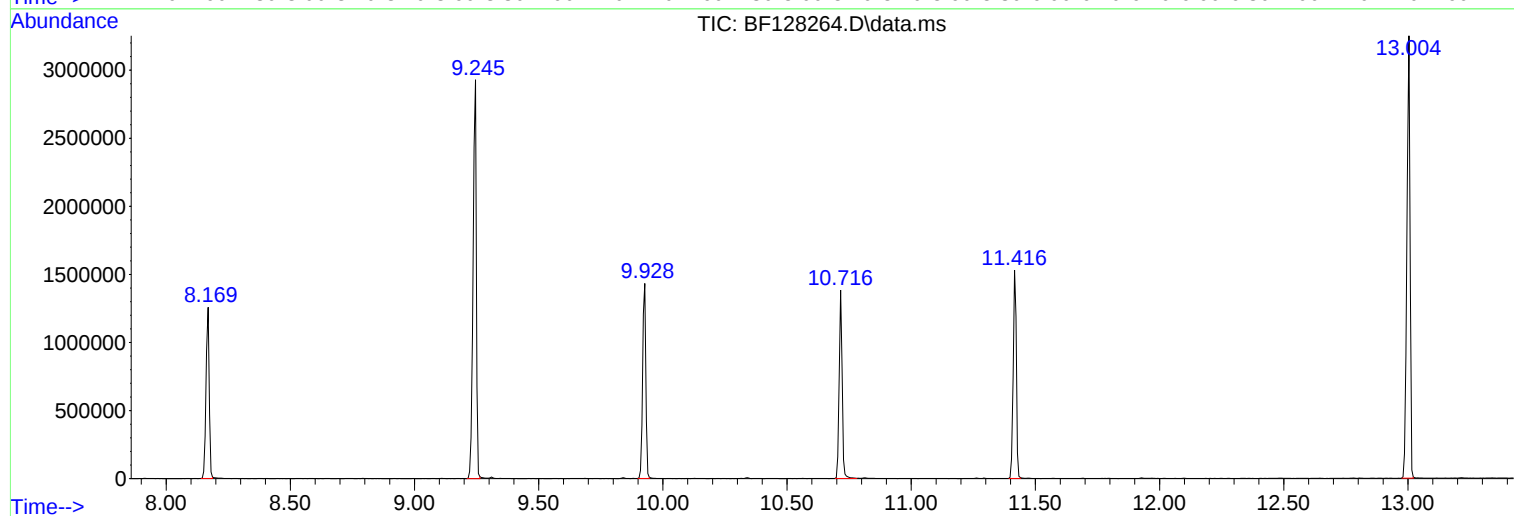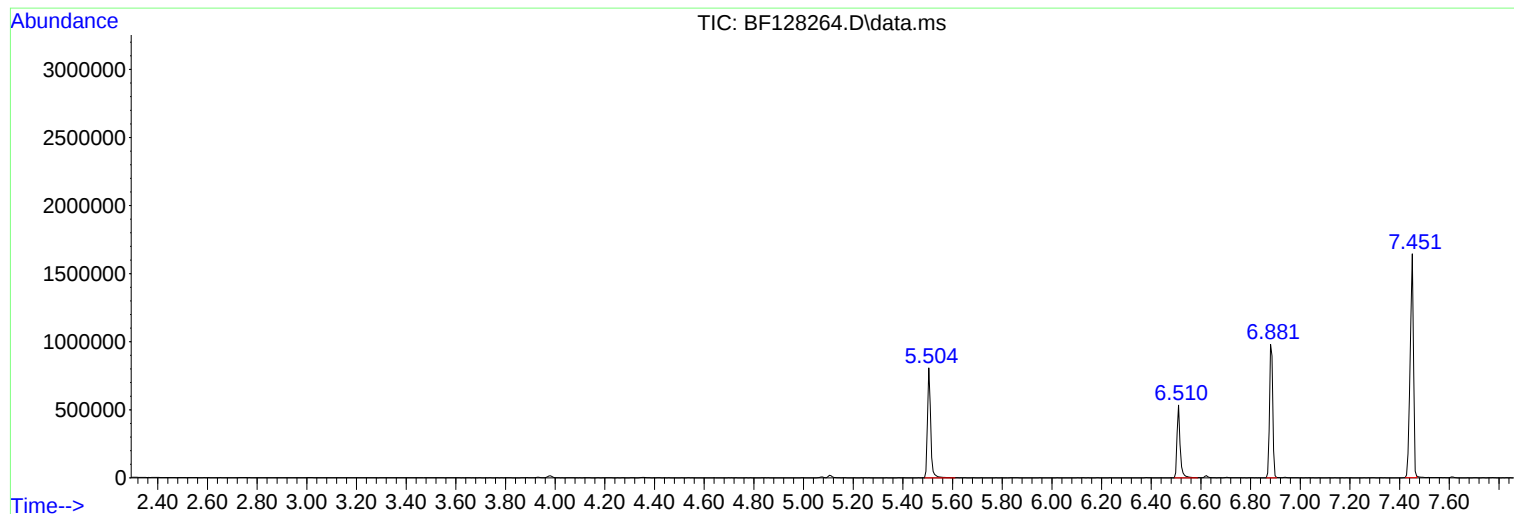

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128264.D
Acq On : 16 May 2022 13:10
Operator : CG\JU
Sample : N2852-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051622\
Data File : BF128264.D
Acq On : 16 May 2022 13:10
Operator : CG\JU
Sample : N2852-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------